


7470A

LB 91461
INSTRUMENT ID: CY1

Linear

 μ Abs.:

3442E

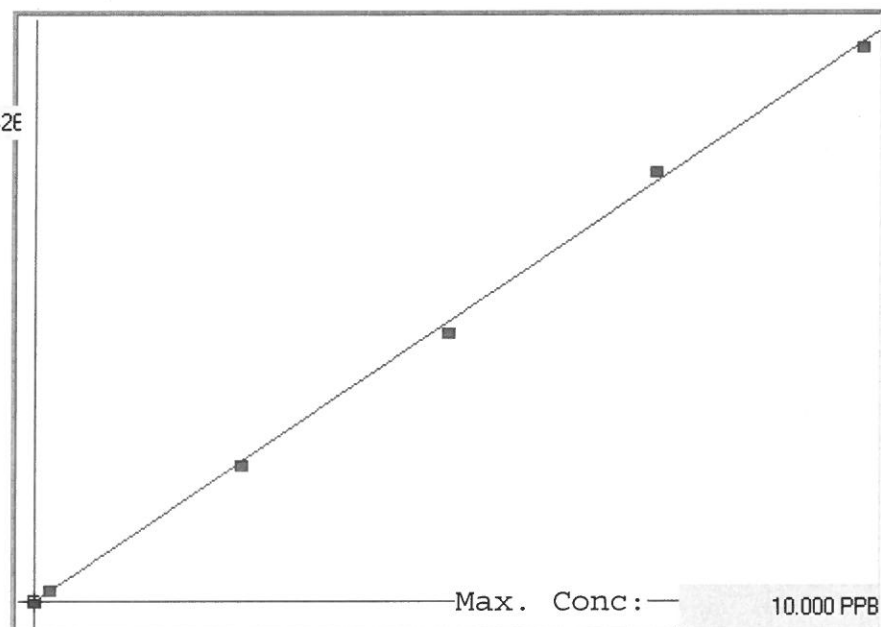

A= 0.0000e+000

B= 2.8777e-004

C= 2.0591e-002

Rho= 0.9994946

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.024	0.024	12	0.000	12				
0.2	0.200	0.246	0.046	782	0.0 %	782				
2.5	2.500	2.463	-0.037	8486	0.0 %	8486				
5.0	5.000	4.830	-0.170	16712	0.0 %	16712				
7.5	7.500	7.710	0.210	26722	0.0 %	26722				
10.0	10.000	9.927	-0.073	34426	0.0 %	34426				

LB91461 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 09 Nov 2017 09:33:03

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	30	12	-	0.0000	7470A	PPB	09 Nov 2017 09:43:37	S	Std
0.2 - 1	50.2	782	-	0.2000	7470A	PPB	09 Nov 2017 09:45:46	S	Std
2.5 - 1	52.5	8486	-	2.5000	7470A	PPB	09 Nov 2017 09:47:54	S	Std
5.0 - 1	55	16712	-	5.0000	7470A	PPB	09 Nov 2017 09:50:02	S	Std
7.5 - 1	57.5	26722	-	7.5000	7470A	PPB	09 Nov 2017 09:52:10	S	Std
10.0 - 1	510	34426	-	10.0000	7470A	PPB	09 Nov 2017 09:54:17	S	Std
ICV54 - 1	ICV54	13762	3.9809	-	7470A	PPB	09 Nov 2017 09:57:02	U	SMPL
ICB54 - 1	ICB54	-118	-0.0134	-	7470A	PPB	09 Nov 2017 09:59:08	U	SMPL
CCV37 - 1	CCV37	16767	4.8457	-	7470A	PPB	09 Nov 2017 10:01:15	U	SMPL
CCB37 - 1	CCB37	-126	-0.0157	-	7470A	PPB	09 Nov 2017 10:03:22	U	SMPL
CRA - 1	CRA	768	0.2416	-	7470A	PPB	09 Nov 2017 10:05:29	U	SMPL
HighStd - 1	HighStd	34575	9.9703	-	7470A	PPB	09 Nov 2017 10:07:36	U	SMPL
ChkStd - 1	ChkStd	24217	6.9896	-	7470A	PPB	09 Nov 2017 10:09:43	U	SMPL
PB104112BL - 1	PBW	-179	-0.0309	-	7470A	PPB	09 Nov 2017 10:11:52	U	SMPL
PB104112BS - 1	LCSW	13586	3.9303	-	7470A	PPB	09 Nov 2017 10:14:01	U	SMPL
PB104112TB - 1	PB104067TB	-88	-0.0047	-	7470A	PPB	09 Nov 2017 10:16:08	U	SMPL
I6304-10 - 1	CL-02-110717	-16	0.0160	-	7470A	PPB	09 Nov 2017 10:18:17	U	SMPL
I6310-04 - 1	1-5-RO	33	0.0301	-	7470A	PPB	09 Nov 2017 10:20:25	U	SMPL
I6310-04DUP - 1	1-5-RODUP	34	0.0304	-	7470A	PPB	09 Nov 2017 10:22:34	U	SMPL
I6310-04MS - 1	1-5-ROMS	12696	3.6741	-	7470A	PPB	09 Nov 2017 10:24:40	U	SMPL
CCV38 - 1	CCV38	16735	4.8365	-	7470A	PPB	09 Nov 2017 10:26:47	U	SMPL
CCB38 - 1	CCB38	-118	-0.0134	-	7470A	PPB	09 Nov 2017 10:28:54	U	SMPL
I6310-04MSD - 1	1-5-ROMSD	12587	3.6428	-	7470A	PPB	09 Nov 2017 10:31:01	U	SMPL
I6373-02 - 1	ROLLOFF-208	-93	-0.0062	-	7470A	PPB	09 Nov 2017 10:33:09	U	SMPL
I6379-03 - 1	TP-1-(2-8)	51	0.0353	-	7470A	PPB	09 Nov 2017 10:35:16	U	SMPL
I6379-06 - 1	TP-2-(1-4)	12	0.0240	-	7470A	PPB	09 Nov 2017 10:37:24	U	SMPL
I6379-09 - 1	TP-3-(1-4)	14	0.0246	-	7470A	PPB	09 Nov 2017 10:39:31	U	SMPL
I6381-02 - 1	RT-4651	21	0.0266	-	7470A	PPB	09 Nov 2017 10:41:39	U	SMPL
I6381-04 - 1	RT-1500	29	0.0289	-	7470A	PPB	09 Nov 2017 10:43:46	U	SMPL
I6310-04LX5 - 1		11	0.0238	-	7470A	PPB	09 Nov 2017 10:45:55	U	SMPL
I6310-04A - 1		14142	4.0903	-	7470A	PPB	09 Nov 2017 10:48:03	U	SMPL
CCV39 - 1	CCV39	16823	4.8618	-	7470A	PPB	09 Nov 2017 10:50:10	U	SMPL
CCB39 - 1	CCB39	-117	-0.0131	-	7470A	PPB	09 Nov 2017 10:52:18	U	SMPL