

Clear table

ident	concentrati on F-	concentrati on CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	date time
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2017-11-01_	11/17/17 12:03
STD2	0.1820	0.2270	0.2500	0.8380	0.1930	0.0920	1.2820	2017-11-01_	11/17/17 12:33
STD3	0.4310	0.6300	0.6330	2.0600	0.5270	1.0560	3.1860	2017-11-01_	11/17/17 13:02
STD4	0.7300	1.2010	1.1780	3.9310	0.9910	2.1530	5.8910	2017-11-01_	11/17/17 13:32
STD5	1.9350	2.8650	2.8590	9.5830	2.3940	5.0530	14.2170	2017-11-01_	11/17/17 14:02
STD6	3.9620	5.9160	5.9100	19.7120	4.9270	9.7640	29.5480	2017-11-01_	11/17/17 14:32
STD7	5.0590	7.6110	7.6200	25.3750	6.3440	12.6310	38.1250	2017-11-01_	11/17/17 15:02
ICV	2.0080	2.8500	2.8540	9.5540	2.3950	5.2660	14.1690	2017-11-01_	11/17/17 16:32
ICB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2017-11-01_	11/17/17 17:02
CCV	2.1270	2.8470	2.8180	9.5030	2.3810	5.1770	13.5890	2017-11-07_	11/17/17 11:20
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2017-11-07_	11/17/17 11:50
LB91486BLS	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2017-11-07_	11/17/17 12:20
LB91486BSS	2.0560	2.8490	2.8250	9.5330	2.3840	5.2850	13.6240	2017-11-07_	11/17/17 12:50
I6298-01	4.0630	43.6450	0.0000	2.7100	10.2850	3.9440	45.7210	2017-11-07_	11/17/17 14:11
I6298-01DLX2	2.0930	20.3060	0.0000	1.5040	4.8720	2.0700	22.7040	2017-11-07_	11/17/17 15:11
I6298-01DLX10	0.4520	3.6300	0.0000	0.5170	0.9660	0.2980	4.7850	2017-11-07_	11/17/17 15:41
CCV	2.0420	2.8630	2.8180	9.5280	2.3830	5.2760	13.6430	2017-11-07_	11/17/17 16:11
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2017-11-07_	11/17/17 16:45


2c-2 / soil 9056
A16
11/13/17

IC-R

11-01-17

CALIBRATION OF COMPONENT F-

Method: AnionsIC2-110117.mtw
Equation: $Q = 0.0175505 \cdot A + 0.604065$
RSD: 3.591 %
Correlation coefficient: 0.999474

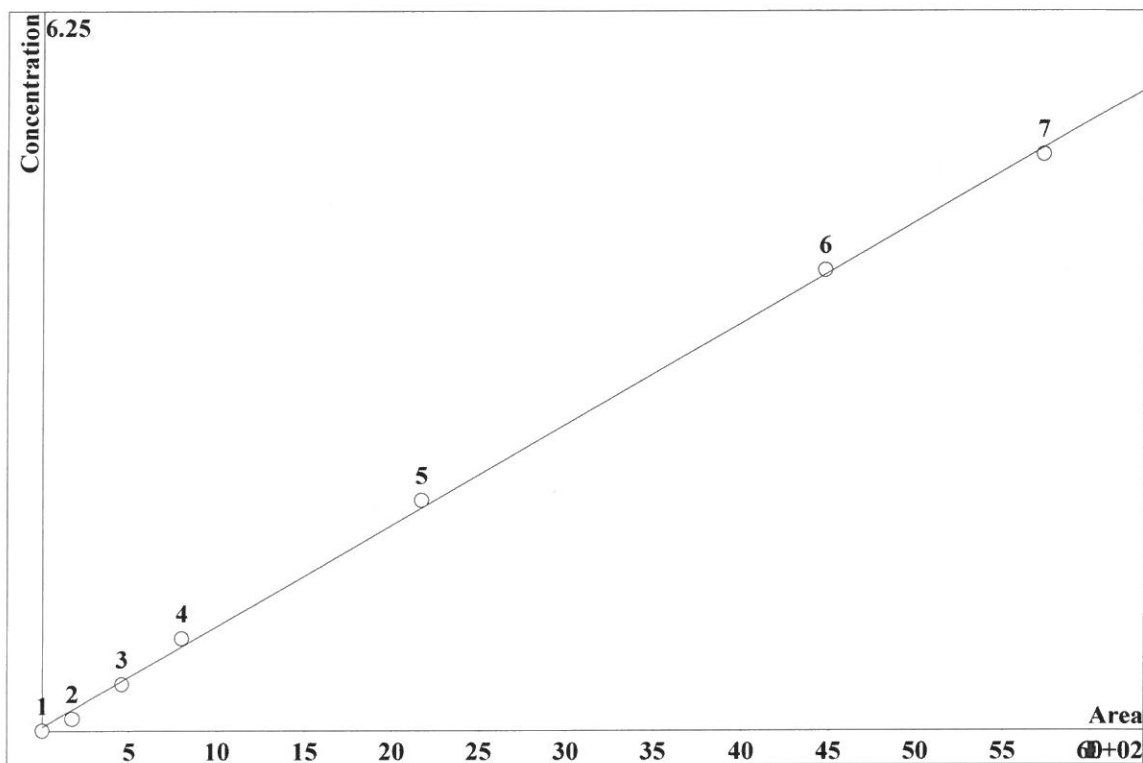


K3 = 0 K2 = 0 K1 = 0.0175505 K0 = 0.604065
Base: Area
Ref.channel: ch1
ISTD:
Formula: Linear
Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		
2	5.803	173.2	0.1	20	5.09		
3	16.27	457.2	0.4	20	5.09		
4	31.78	797.3	0.8	20	5.09		
5	75.45	2171	2	20	5.09		
6	163.7	4481	4	20	5.09		
7	202.7	5730	5	20	5.09		

1.□

CALIBRATION OF COMPONENT CL-

Method: AnionsIC2-110117.mtw
 Equation: $Q = 0.0266871 \cdot A + 1.5137$
 RSD: 3.438 %
 Correlation coefficient: 0.999517

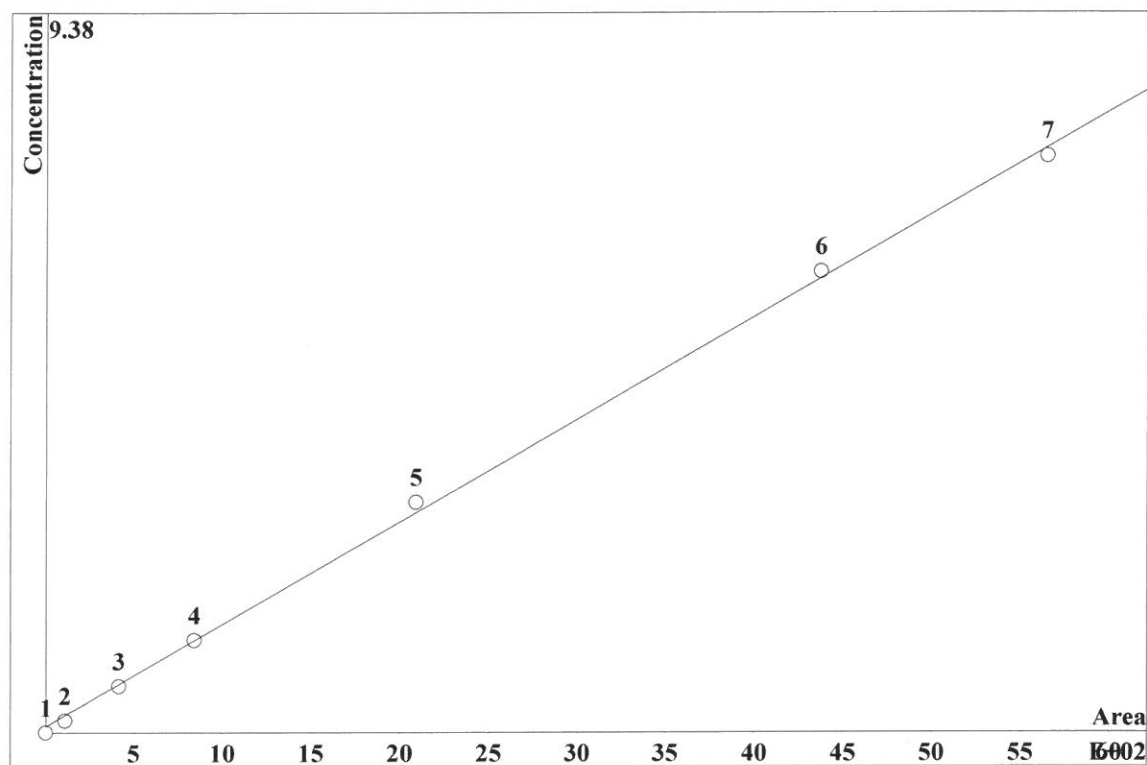


K3 = 0 K2 = 0 K1 = 0.0266871 K0 = 1.5137
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	6.042	113.6	0.15	20	8.696		
3	23.02	415.4	0.6	20	8.696		
4	46.99	843.2	1.2	20	8.696		
5	119.6	2090	3	20	8.696		
6	254.3	4377	6	20	8.696		
7	327.3	5647	7.5	20	8.696		

CALIBRATION OF COMPONENT NO2

Method: AnionsIC2-110117.mtw
 Equation: $Q = 0.0112803 \cdot A + 2.78394$
 RSD: 3.789 %
 Correlation coefficient: 0.999414

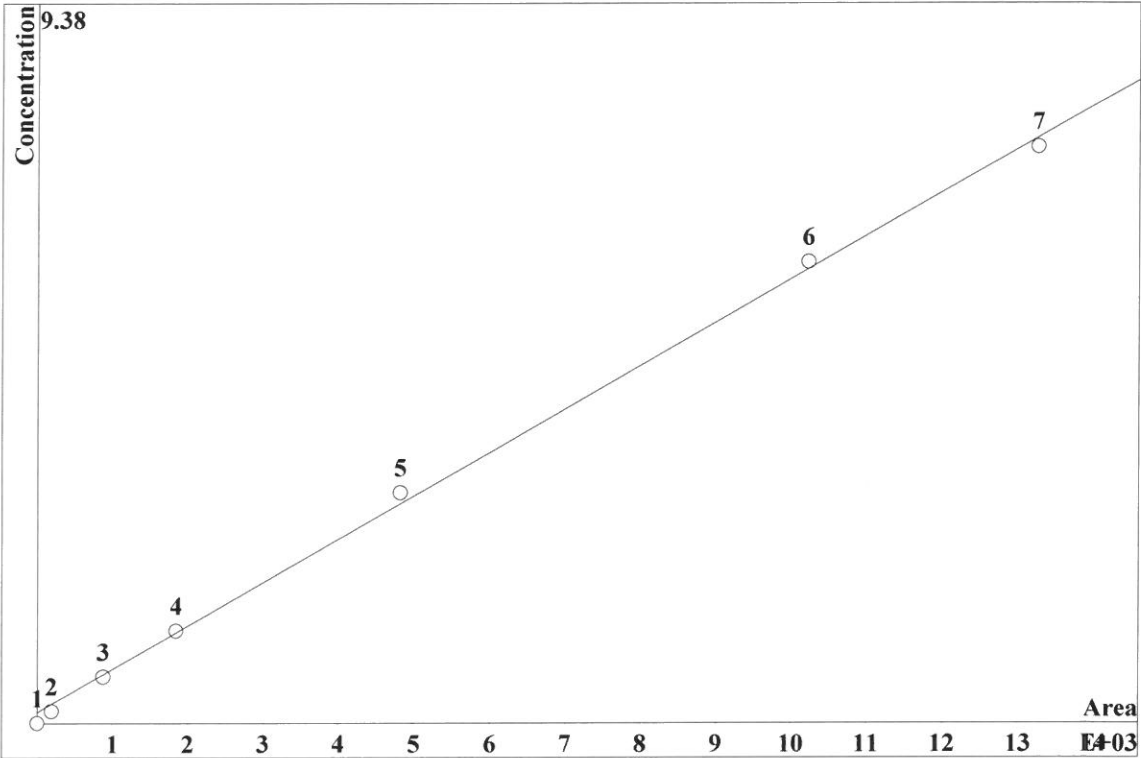


K3 = 0 K2 = 0 K1 = 0.0112803 K0 = 2.78394
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	9.45	197	0.15	20	11.13		
3	41.14	875.5	0.6	20	11.13		
4	87.02	1842	1.2	20	11.13		
5	228.8	4822	3	20	11.13		
6	485.6	1.023e+04	6	20	11.13		
7	628.3	1.326e+04	7.5	20	11.13		

CALIBRATION OF COMPONENT BR-

Method: AnionsIC2-110117.mtw
 Equation: $Q = 0.0601743 \cdot A + 5.34617$
 RSD: 3.517 %
 Correlation coefficient: 0.999495

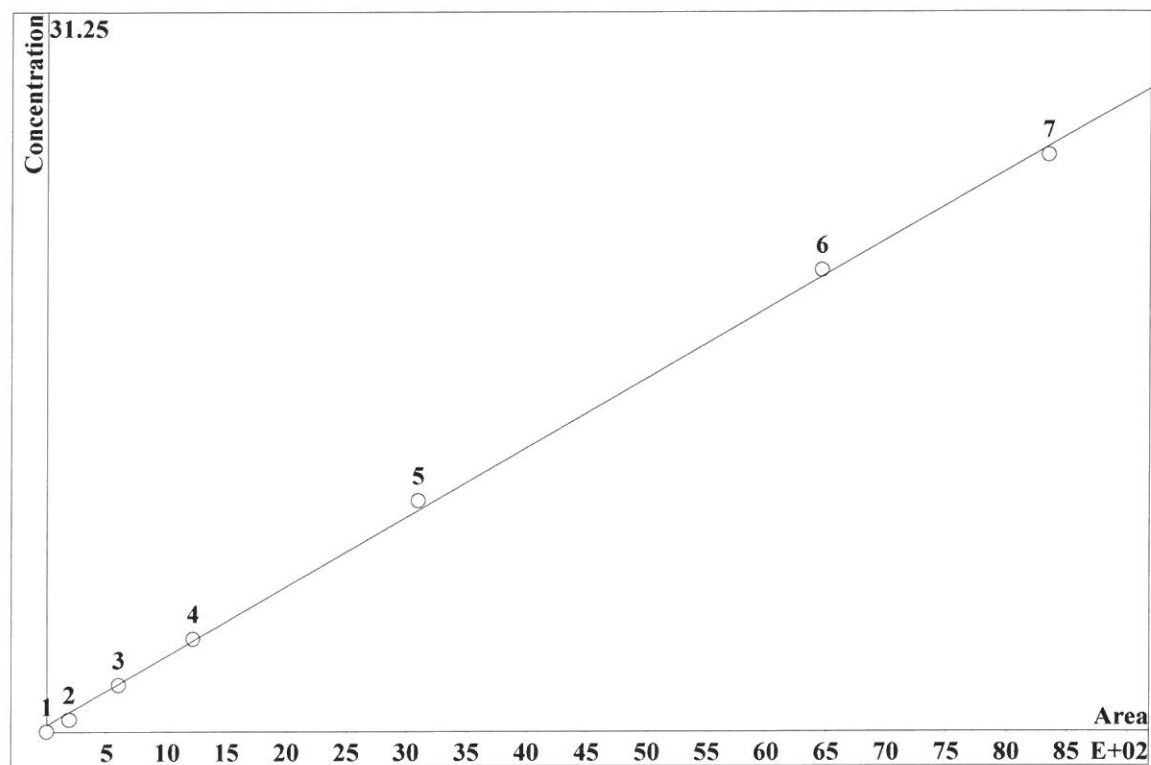


K3 = 0 K2 = 0 K1 = 0.0601743 K0 = 5.34617
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	5.52	189.7	0.5	20	14.57		
3	20.87	595.7	2	20	14.57		
4	42.92	1218	4	20	14.57		
5	109.9	3096	10	20	14.57		
6	231.6	6463	20	20	14.57		
7	297.7	8345	25	20	14.57		

CALIBRATION OF COMPONENT NO3

Method: AnionsIC2-110117.mtw
 Equation: $Q = 0.010691 \cdot A + 1.83826$
 RSD: 3.432 %
 Correlation coefficient: 0.999519

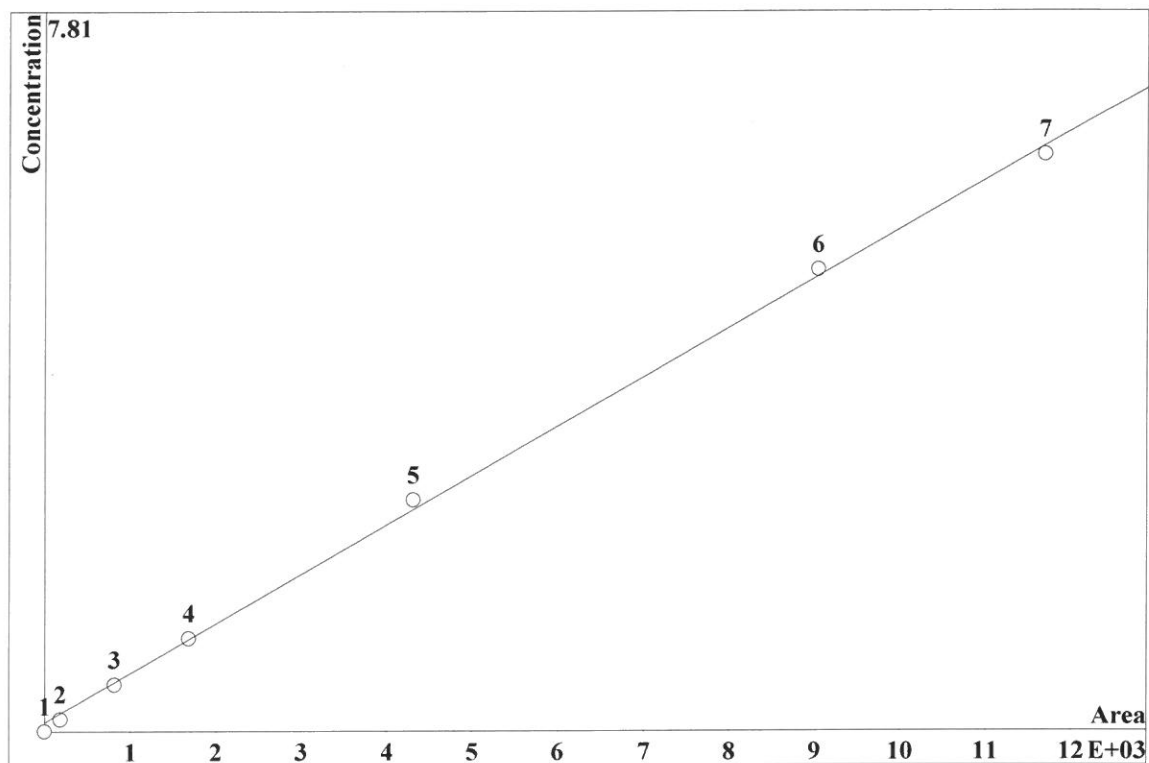


K3 = 0 K2 = 0 K1 = 0.010691 K0 = 1.83826
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	5.629	188.9	0.125	20	17.32		
3	24	813.1	0.5	20	17.32		
4	49.63	1682	1	20	17.32		
5	127.2	4306	2.5	20	17.32		
6	266.2	9044	5	20	17.32		
7	341	1.17e+04	6.25	20	17.32		

CALIBRATION OF COMPONENT HPO4

Method: AnionsIC2-110117.mtw
 Equation: $Q = 0.0339608 \cdot A - 11.3175$
 RSD: 3.479 %
 Correlation coefficient: 0.999506

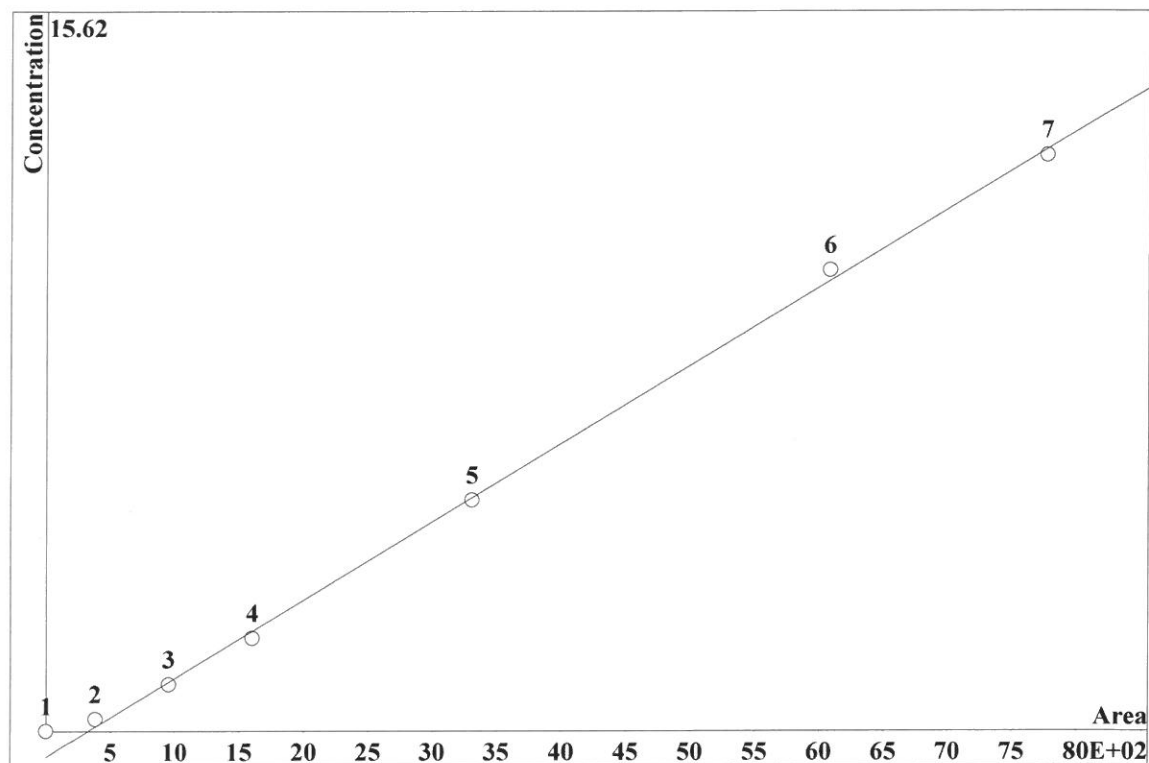


K3 = 0 K2 = 0 K1 = 0.0339608 K0 = -11.3175
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	6.764	387.5	0.25	20	22.67		
3	16.97	955	1	20	22.67		
4	29.29	1601	2	20	22.67		
5	61.29	3309	5	20	22.67		
6	114.7	6084	10	20	22.67		
7	146	7772	12.5	20	22.67		

CALIBRATION OF COMPONENT SO4

Method: AnionsIC2-110117.mtw
 Equation: $Q = 0.0368229 \cdot A + 13.4507$
 RSD: 4.033 %
 Correlation coefficient: 0.999336

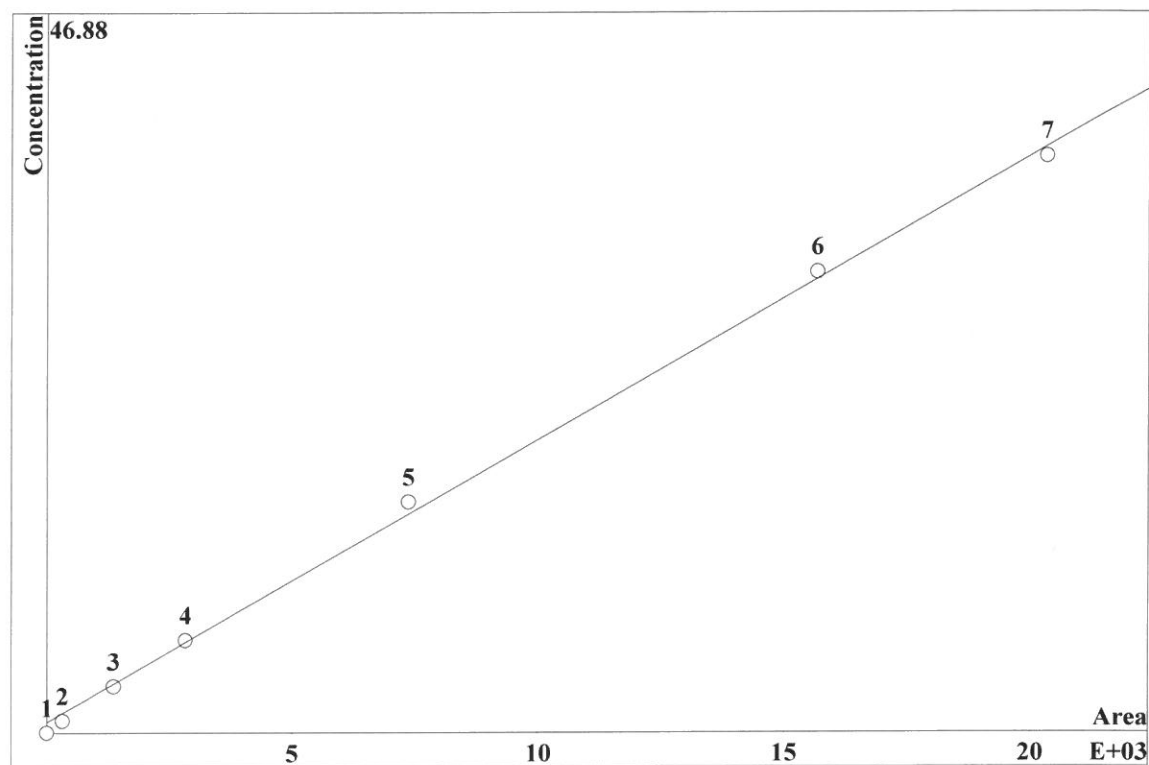

K3 = 0 K2 = 0 K1 = 0.0368229 K0 = 13.4507
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	6.9	331.3	0.75	20	24.48		
3	27.61	1365	3	20	24.48		
4	57.18	2834	6	20	24.48		
5	145.8	7357	15	20	24.48		
6	308	1.568e+04	30	20	24.48		
7	395.2	2.034e+04	37.5	20	24.48		

Report date: 11/1/2017 6:07:42 PM
Printed by: wet


Ident: STD1
Analysis from: 11/1/2017 12:03:07 PM
File: _2017-11-01_

Last save: 11/1/2017 4:19:34 PM

Method: AnionsIC2-110117.mtw
Run operator: wet
Analysis number: 15626

Last save: 11/1/2017 2:59:

SAMPLE:
: AK/AP
Vial number: 2
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

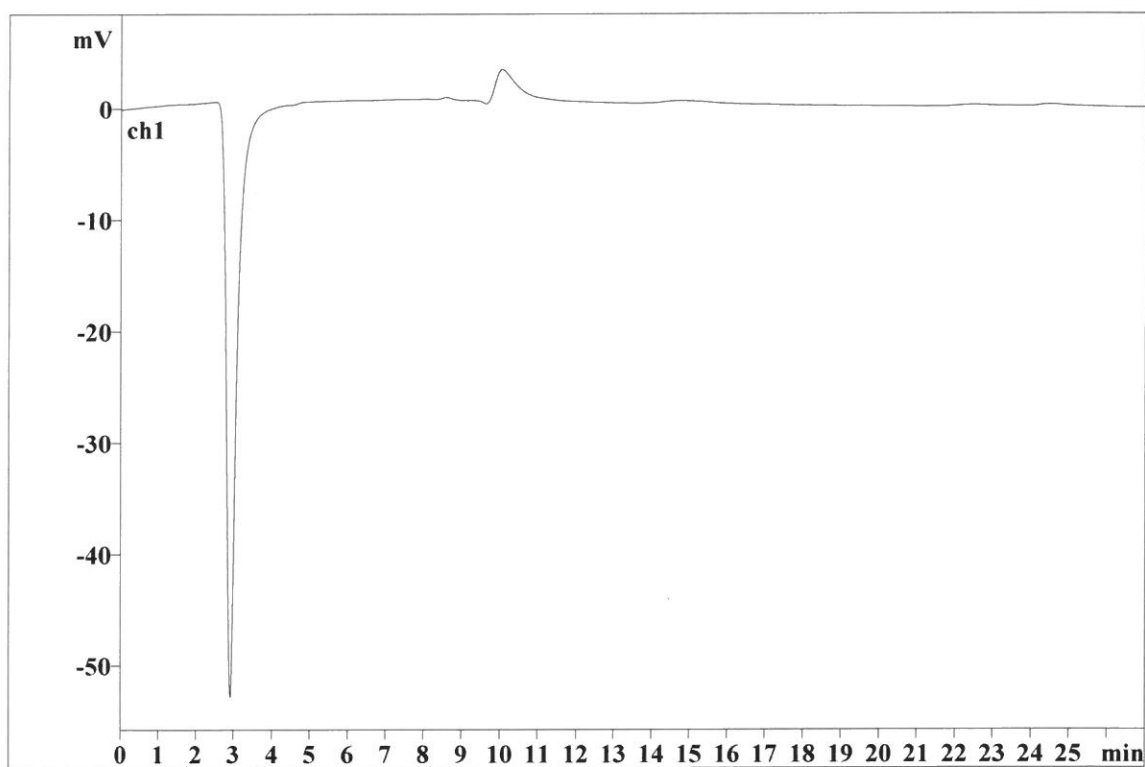

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 11/1/2017 6:07:49 PM
Printed by: wet


Ident: STD2
Analysis from: 11/1/2017 12:33:02 PM
File: _2017-11-01_

Last save: 11/1/2017 4:19:34 PM

Method: AnionsIC2-110117.mtw
Run operator: wet
Analysis number: 15627

Last save: 11/1/2017 2:59:

SAMPLE:
: AK/AP
Vial number: 3
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

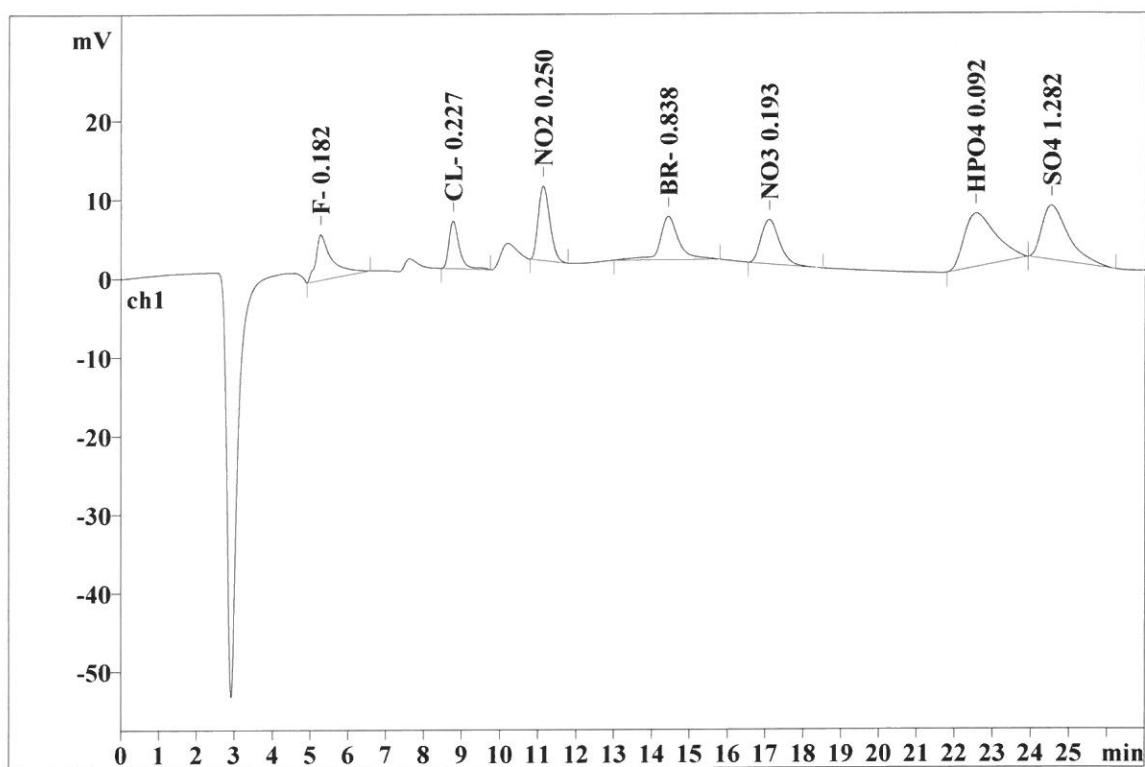

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.27	0.361	5.80	12.58	173.210	10.95
2	8.77	0.270	6.04	13.10	113.629	7.19
3	11.14	0.326	9.45	20.49	197.026	12.46
4	14.45	0.457	5.52	11.97	189.734	12.00
5	17.11	0.520	5.63	12.21	188.918	11.95
6	22.57	0.899	6.76	14.67	387.482	24.50
7	24.55	0.709	6.90	14.96	331.295	20.95
7	27.00	0.506	46.10	99.98	1581.294	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/1/2017 6:07:55 PM
Printed by: wet


Ident: STD3
Analysis from: 11/1/2017 1:02:58 PM
File: _2017-11-01_

Last save: 11/1/2017 4:19:34 PM

Method: AnionsIC2-110117.mtw
Run operator: wet
Analysis number: 15628

Last save: 11/1/2017 2:59:

SAMPLE:
: AK/AP
Vial number: 4
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

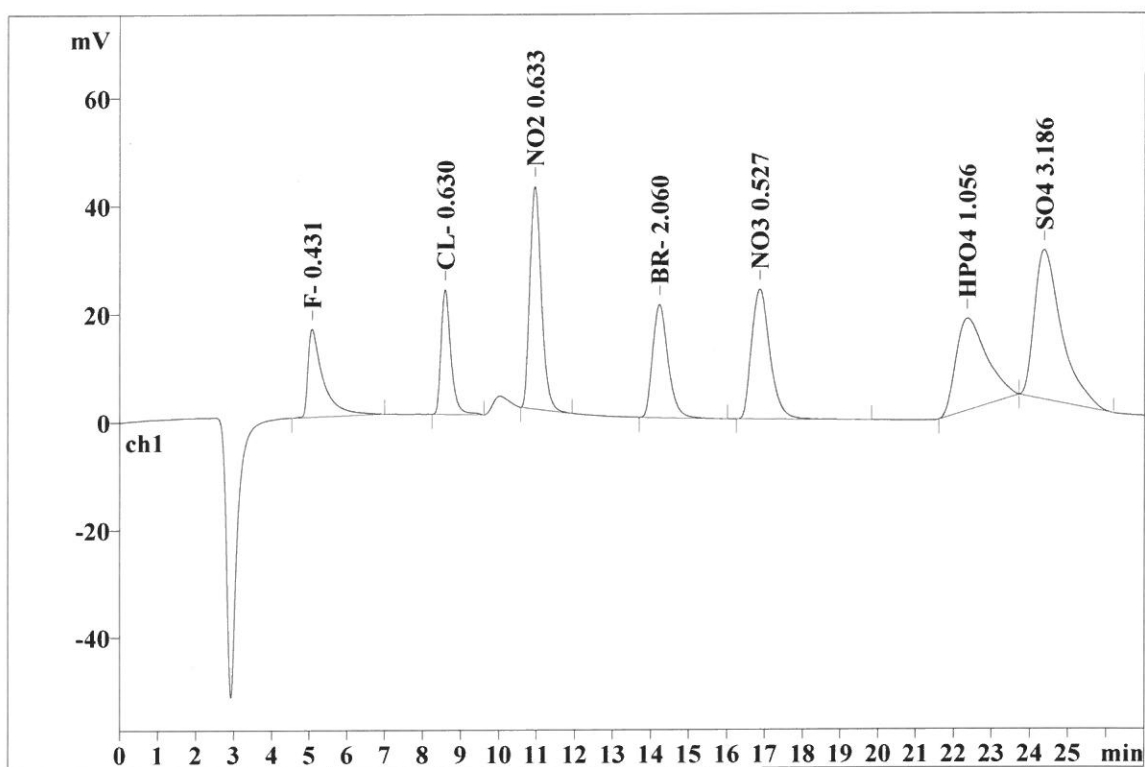

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.08	0.363	16.27	9.58	457.225	8.35
2	8.60	0.266	23.01	13.55	415.387	7.58
3	10.96	0.327	41.14	24.22	875.454	15.98
4	14.24	0.437	20.87	12.29	595.746	10.88
5	16.88	0.519	24.00	14.13	813.120	14.85
6	22.36	0.877	16.97	9.99	955.042	17.44
7	24.39	0.723	27.61	16.25	1365.063	24.92
7	27.00	0.502	169.88	100.00	5477.037	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/1/2017 6:08:01 PM
Printed by: wet


Ident: STD4
Analysis from: 11/1/2017 1:32:54 PM
File: _2017-11-01_

Last save: 11/1/2017 4:19:34 PM

Method: AnionsIC2-110117.mtw
Run operator: wet
Analysis number: 15629

Last save: 11/1/2017 2:59:

SAMPLE:
: AK/AP
Vial number: 5
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

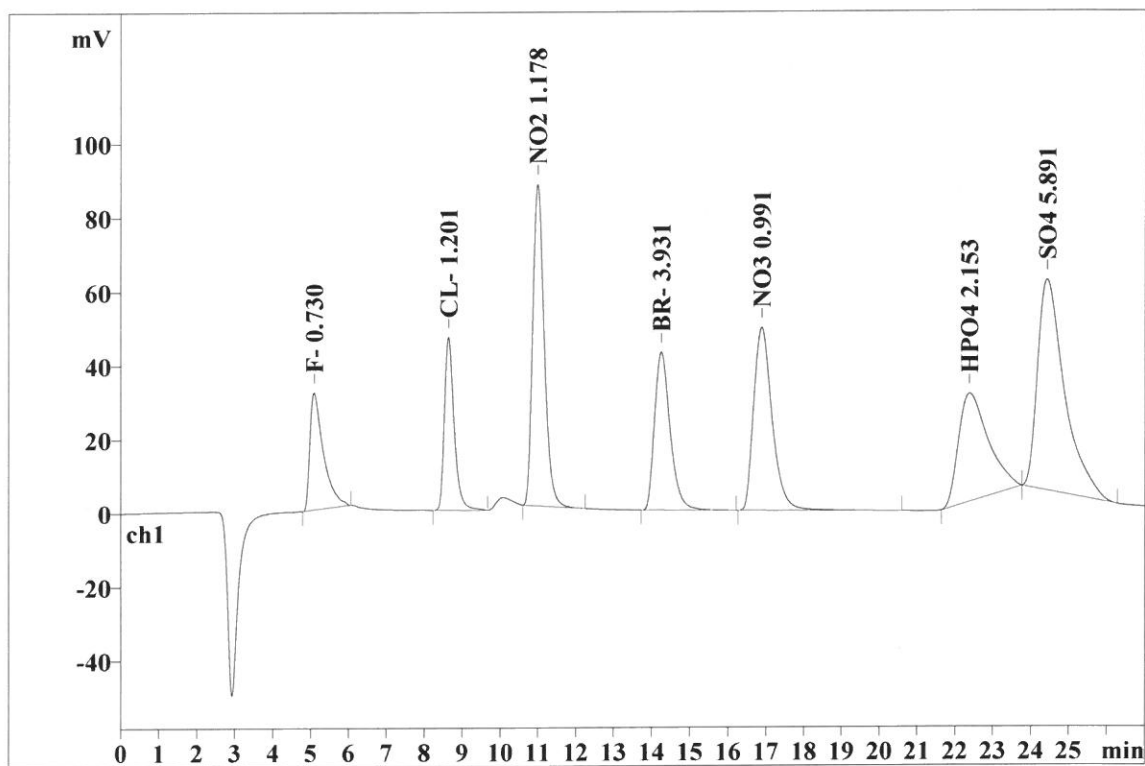

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.09	0.361	31.78	9.22	797.337	7.37
2	8.64	0.264	46.99	13.63	843.237	7.80
3	11.00	0.323	87.02	25.24	1841.636	17.03
4	14.26	0.432	42.92	12.45	1217.616	11.26
5	16.89	0.515	49.63	14.39	1681.773	15.55
6	22.39	0.842	29.29	8.49	1601.269	14.80
7	24.45	0.722	57.18	16.58	2834.180	26.20
7	27.00	0.494	344.81	100.00	10817.049	100.00

Report date: 11/1/2017 6:08:07 PM
Printed by: wet


Ident: STD5
Analysis from: 11/1/2017 2:02:49 PM
File: _2017-11-01_

Last save: 11/1/2017 4:19:35 PM

Method: AnionsIC2-110117.mtw
Run operator: wet
Analysis number: 15630

Last save: 11/1/2017 2:59:

SAMPLE:
: AK/AP
Vial number: 6
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

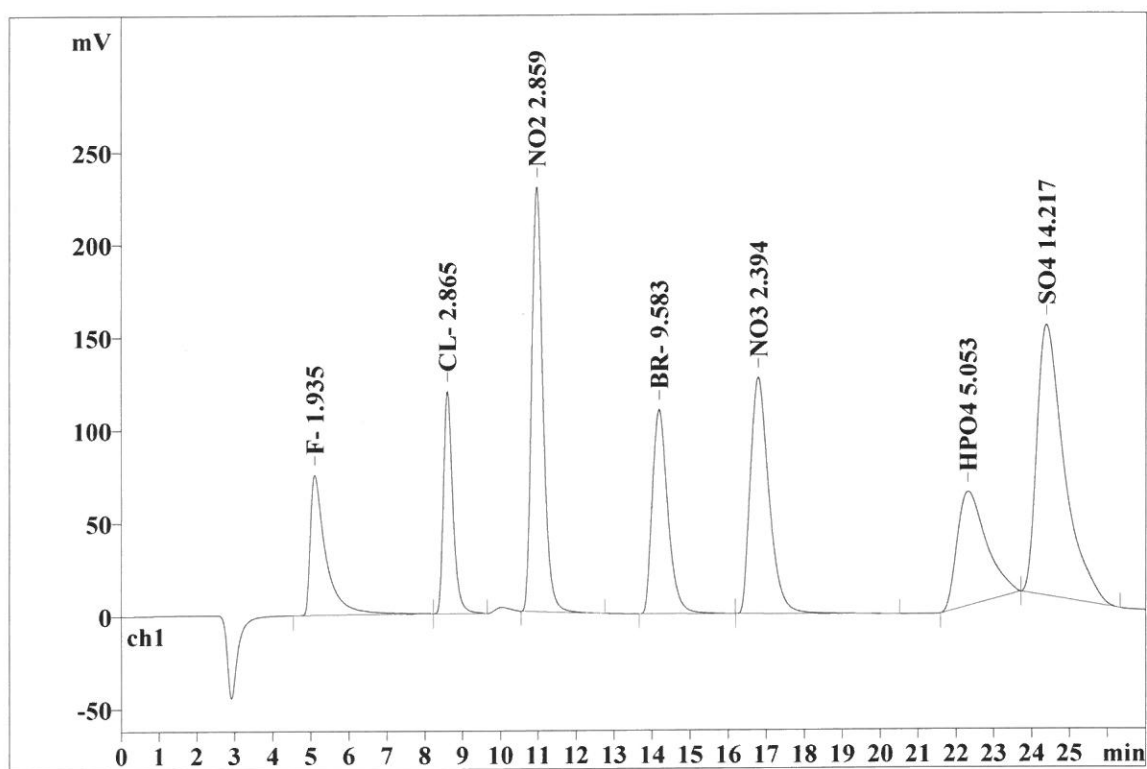

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.10	0.376	75.45	8.69	2171.158	8.00
2	8.60	0.259	119.64	13.78	2090.058	7.70
3	10.97	0.319	228.83	26.36	4821.686	17.76
4	14.19	0.427	109.85	12.66	3096.399	11.40
5	16.80	0.514	127.15	14.65	4306.202	15.86
6	22.32	0.827	61.29	7.06	3309.318	12.19
7	24.40	0.735	145.79	16.80	7356.679	27.09
7	27.00	0.494	868.00	100.00	27151.501	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/1/2017 6:08:13 PM
Printed by: wet


Ident: STD6
Analysis from: 11/1/2017 2:32:45 PM
File: _2017-11-01_

Last save: 11/1/2017 4:19:35 PM

Method: AnionsIC2-110117.mtw
Run operator: wet
Analysis number: 15631

Last save: 11/1/2017 2:59:

SAMPLE:
: AK/AP
Vial number: 7
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

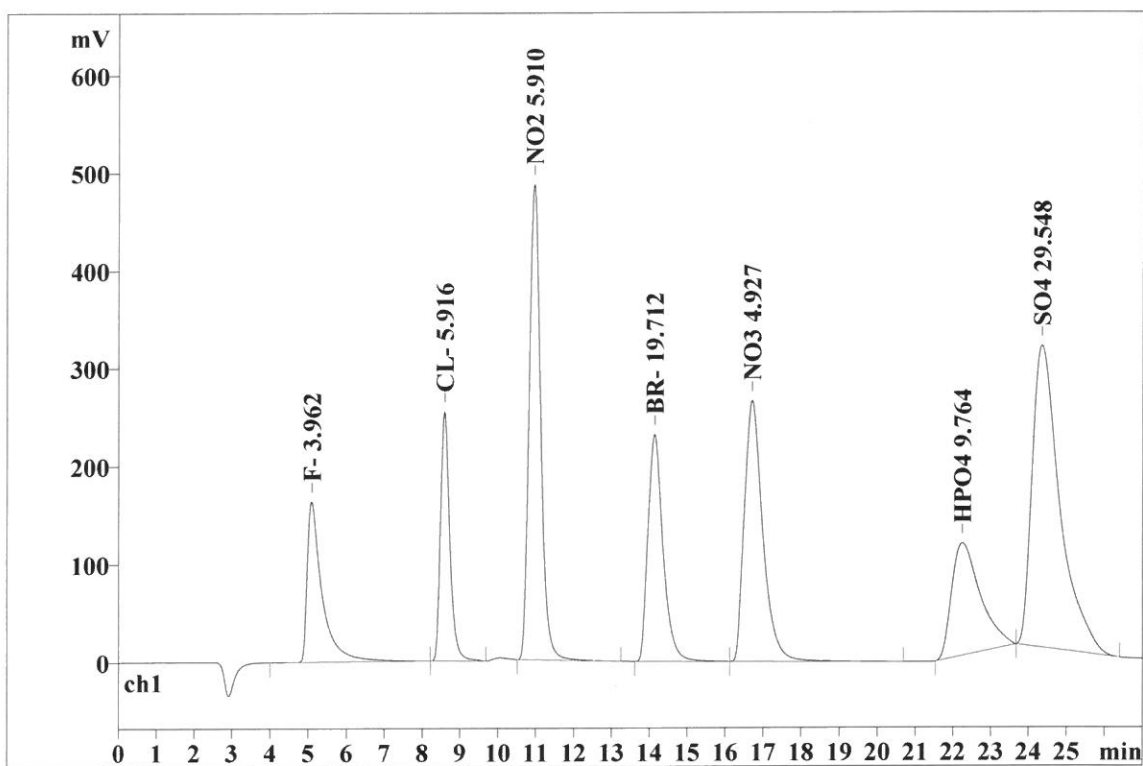

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.09	0.358	163.72	8.98	4481.025	7.95
2	8.59	0.255	254.25	13.94	4376.774	7.77
3	10.96	0.319	485.55	26.62	10230.922	18.15
4	14.14	0.423	231.59	12.70	6462.951	11.47
5	16.72	0.515	266.23	14.60	9044.412	16.05
6	22.25	0.808	114.66	6.29	6083.554	10.79
7	24.36	0.741	308.03	16.89	15683.689	27.83
7	27.00	0.488	1824.05	100.00	56363.325	100.00

Report date: 11/1/2017 6:08:24 PM
Printed by: wet


Ident: STD7
Analysis from: 11/1/2017 3:02:41 PM
File: _2017-11-01_

Last save: 11/1/2017 4:21:19 PM

Method: AnionsIC2-110117.mtw
Run operator: wet
Analysis number: 15632

Last save: 11/1/2017 2:59:

SAMPLE:
: AK/AP
Vial number: 8
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

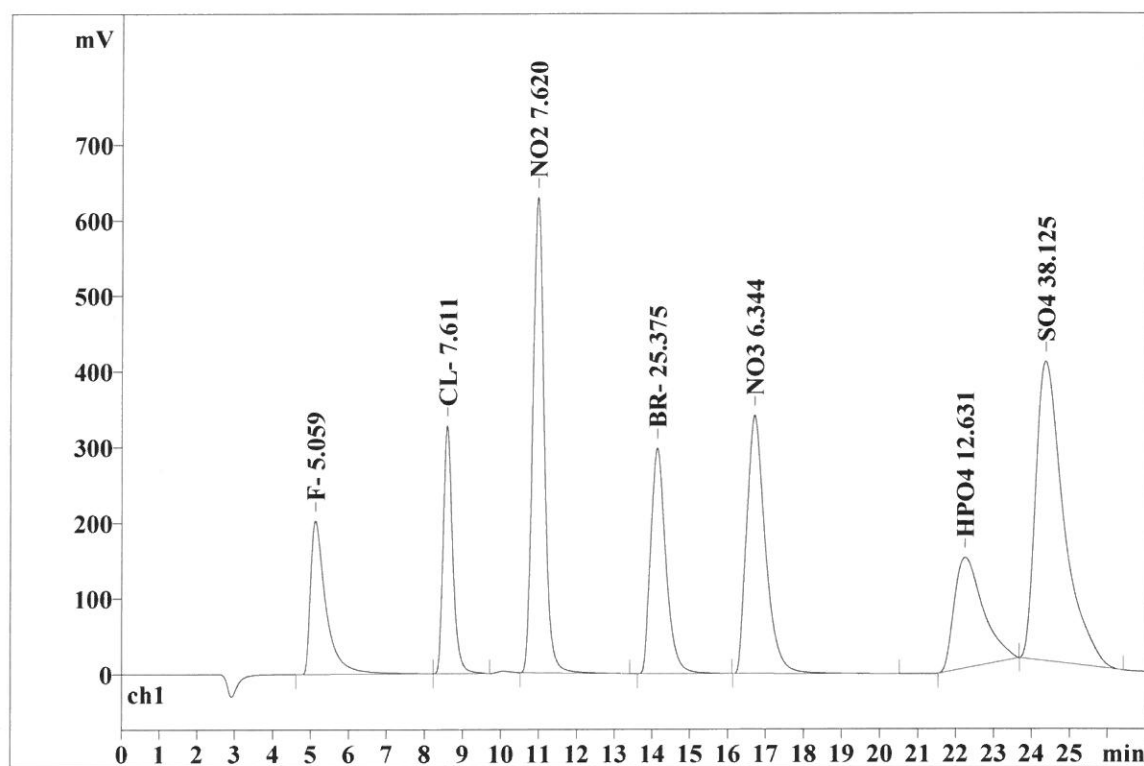

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.12	0.385	202.71	8.67	5730.194	7.87
2	8.59	0.255	327.29	14.00	5647.485	7.76
3	10.97	0.319	628.25	26.87	13264.293	18.22
4	14.13	0.425	297.73	12.73	8345.113	11.46
5	16.70	0.520	341.01	14.58	11696.334	16.07
6	22.24	0.810	146.00	6.24	7771.975	10.68
7	24.37	0.750	395.21	16.90	20342.102	27.94
7	27.00	0.495	2338.20	100.00	72797.496	100.00

Report date: 11/1/2017 6:08:58 PM
Printed by: wet


Ident: ICV
Analysis from: 11/1/2017 4:32:34 PM
File: _2017-11-01_

Last save: 11/1/2017 4:59:34 PM

Method: AnionsIC2-110117.mtw
Run operator: wet
Analysis number: 15635

Last save: 11/1/2017 4:19:

SAMPLE:
: AK/AP
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

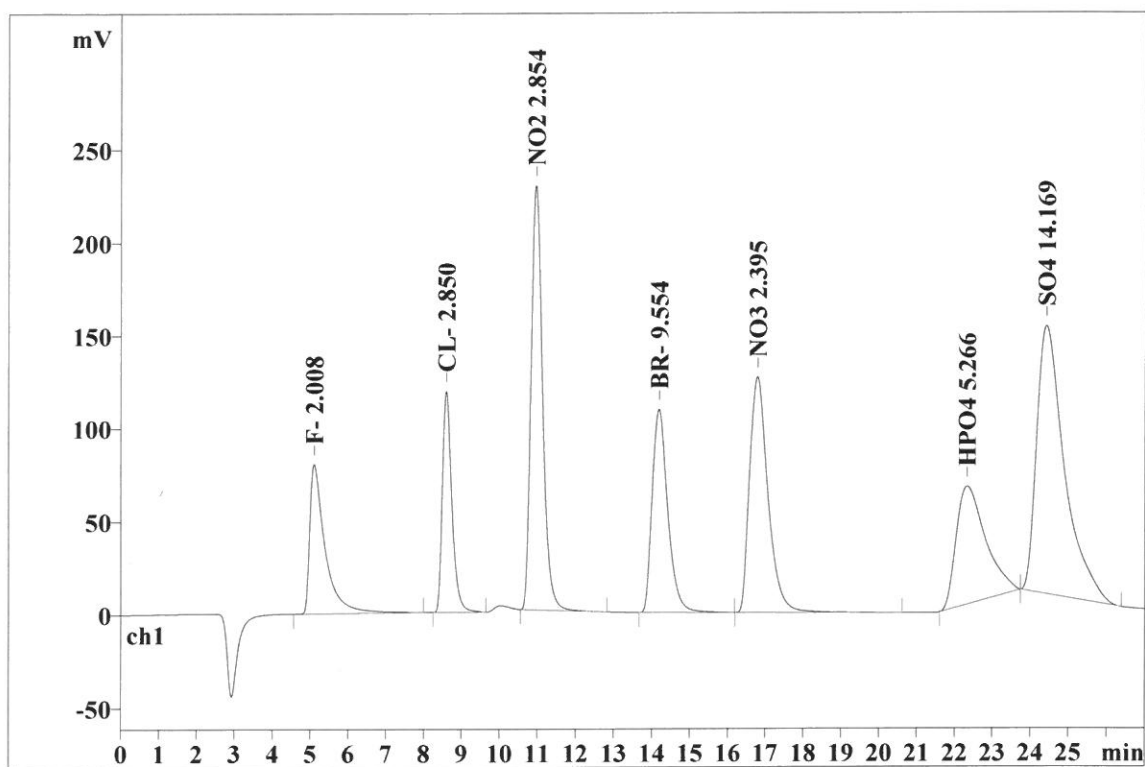

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.11	0.374	80.22	9.22	2254.191	8.26
2	8.60	0.260	118.65	13.63	2079.252	7.61
3	10.97	0.320	228.30	26.23	4813.228	17.63
4	14.19	0.430	109.06	12.53	3086.604	11.30
5	16.80	0.517	126.55	14.54	4308.417	15.78
6	22.33	0.830	63.34	7.28	3434.504	12.58
7	24.43	0.738	144.23	16.57	7330.695	26.85
7	27.00	0.496	870.35	100.00	27306.891	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/1/2017 6:09:07 PM
Printed by: wet


Ident: ICB
Analysis from: 11/1/2017 5:02:30 PM
File: _2017-11-01_

Last save: 11/1/2017 5:29:30 PM

Method: AnionsIC2-110117.mtw
Run operator: wet
Analysis number: 15636

Last save: 11/1/2017 4:19:

SAMPLE:
: AK/AP
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

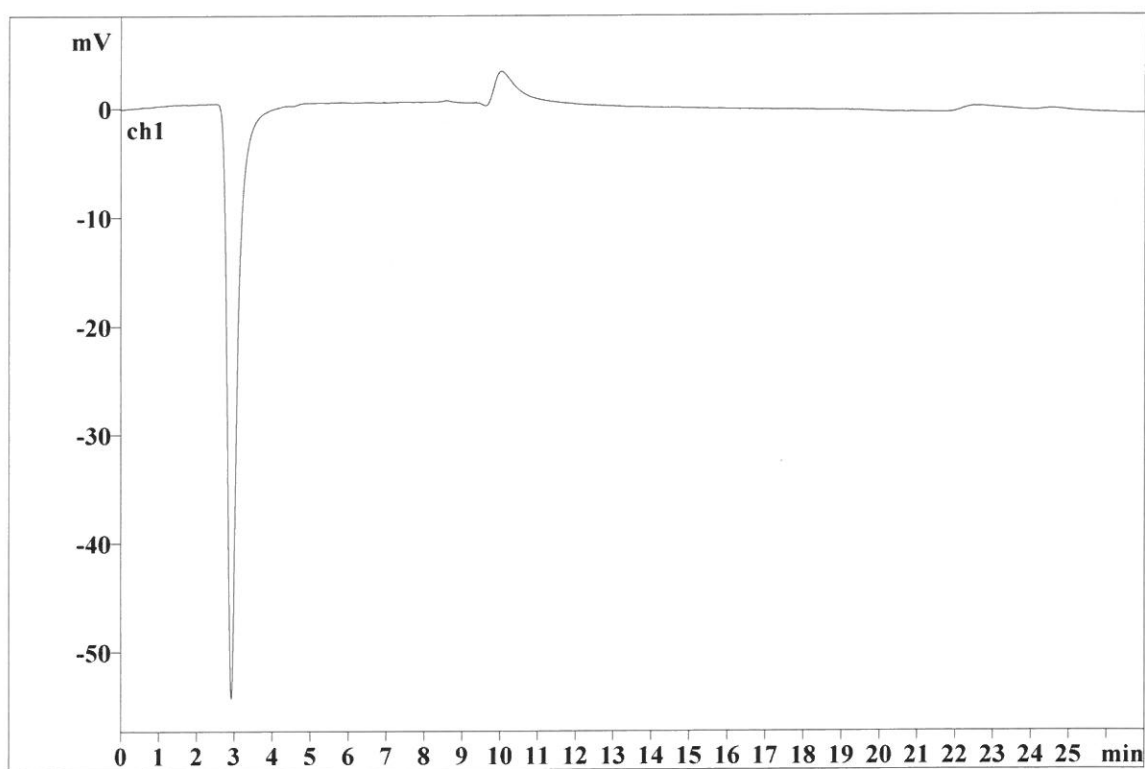

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 11/13/2017 11:32:13 AM
Printed by: wet


Ident: CCV
Analysis from: 11/7/2017 11:20:19 AM
File: _2017-11-07_

Last save: 11/7/2017 11:47:19 AM

Method: AnionsIC2-110117.mtw
Run operator: wet
Analysis number: 15697

Last save: 11/1/2017 3:19:

SAMPLE:
: AK/AP
Vial number: 2
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

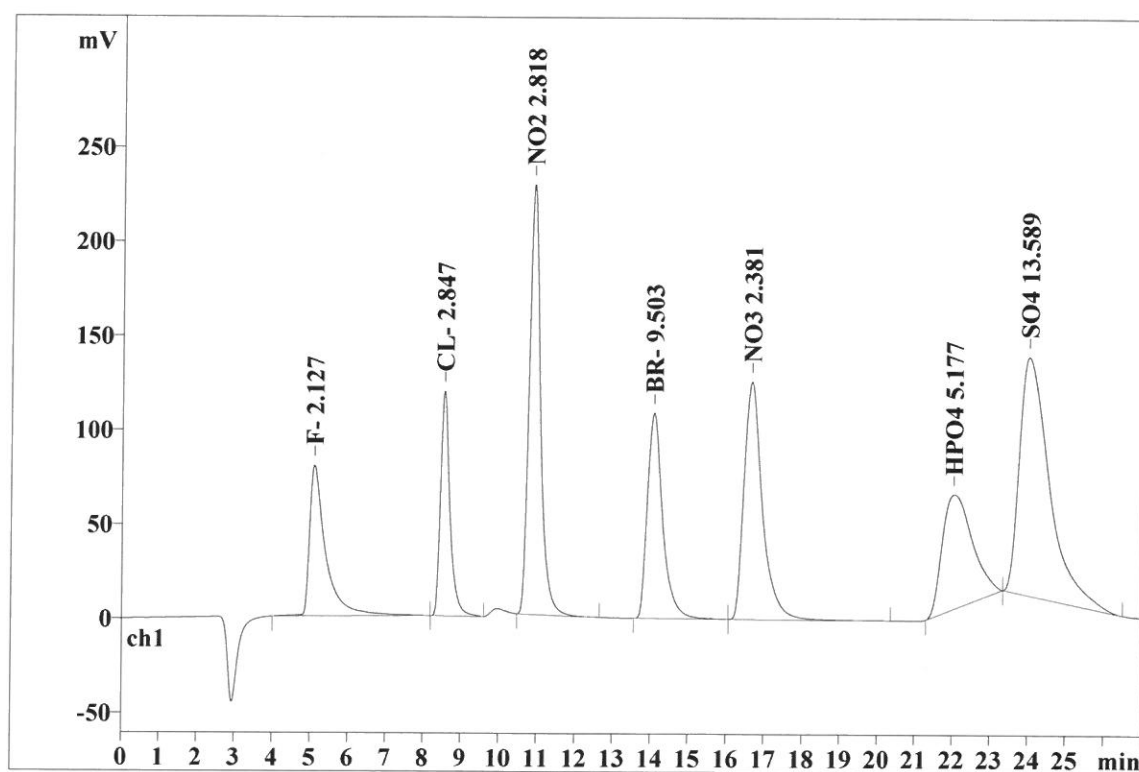

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.09	0.388	79.97	9.42	2389.546	8.86
2	8.54	0.250	119.19	14.04	2076.617	7.70
3	10.89	0.307	227.94	26.85	4749.002	17.61
4	14.07	0.413	108.87	12.82	3069.760	11.38
5	16.64	0.498	125.87	14.82	4282.524	15.88
6	22.01	0.878	60.77	7.16	3381.836	12.54
7	24.01	0.809	126.42	14.89	7015.569	26.02
7	27.00	0.506	849.02	100.00	26964.855	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/13/2017 11:33:02 AM
Printed by: wet


Ident: CCB
Analysis from: 11/7/2017 11:50:54 AM
File: _2017-11-07_

Last save: 11/13/2017 11:32:51 AM

Method: AnionsIC2-110117.mtw
Run operator: wet
Analysis number: 15698

Last save: 11/1/2017 3:19:

SAMPLE:
: AK/AP
Vial number: 3
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

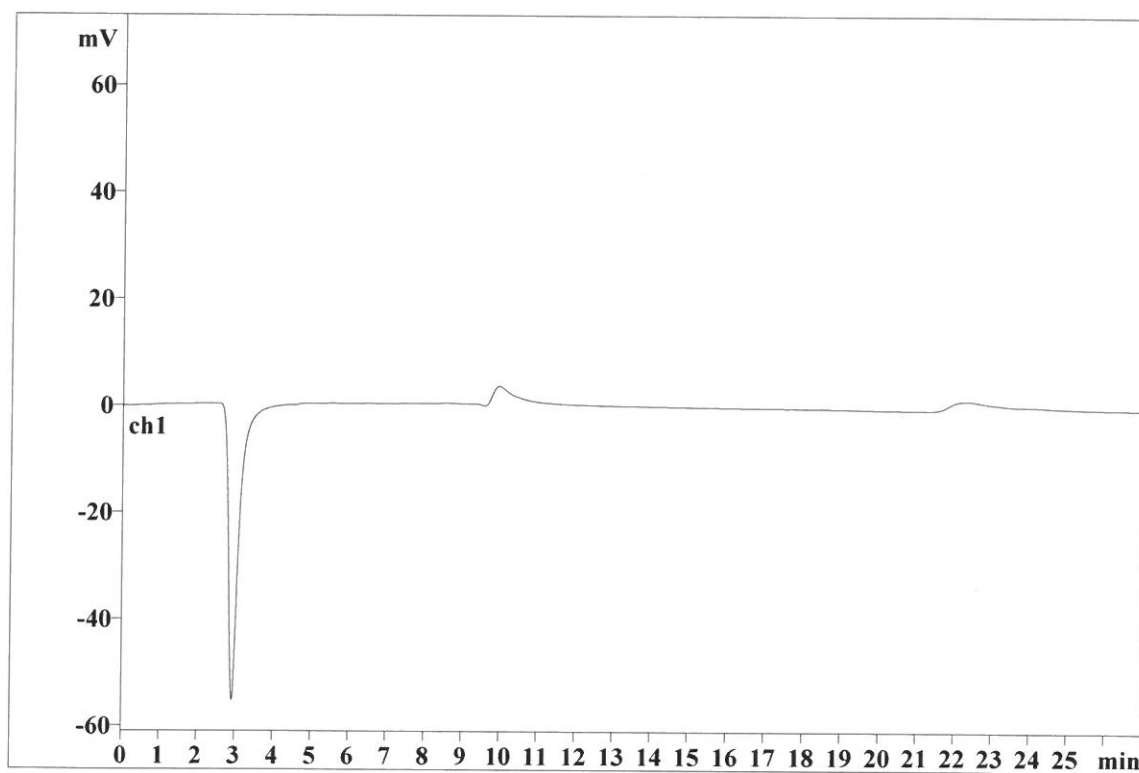

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 11/13/2017 11:33:12 AM
Printed by: wet


Ident: LB91486BLS
Analysis from: 11/7/2017 12:20:50 PM
File: _2017-11-07_

Last save: 11/13/2017 11:32:51 AM

Method: AnionsIC2-110117.mtw
Run operator: wet
Analysis number: 15699

Last save: 11/1/2017 3:19:

SAMPLE: 5.01g
: AK/AP
Vial number: 4
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

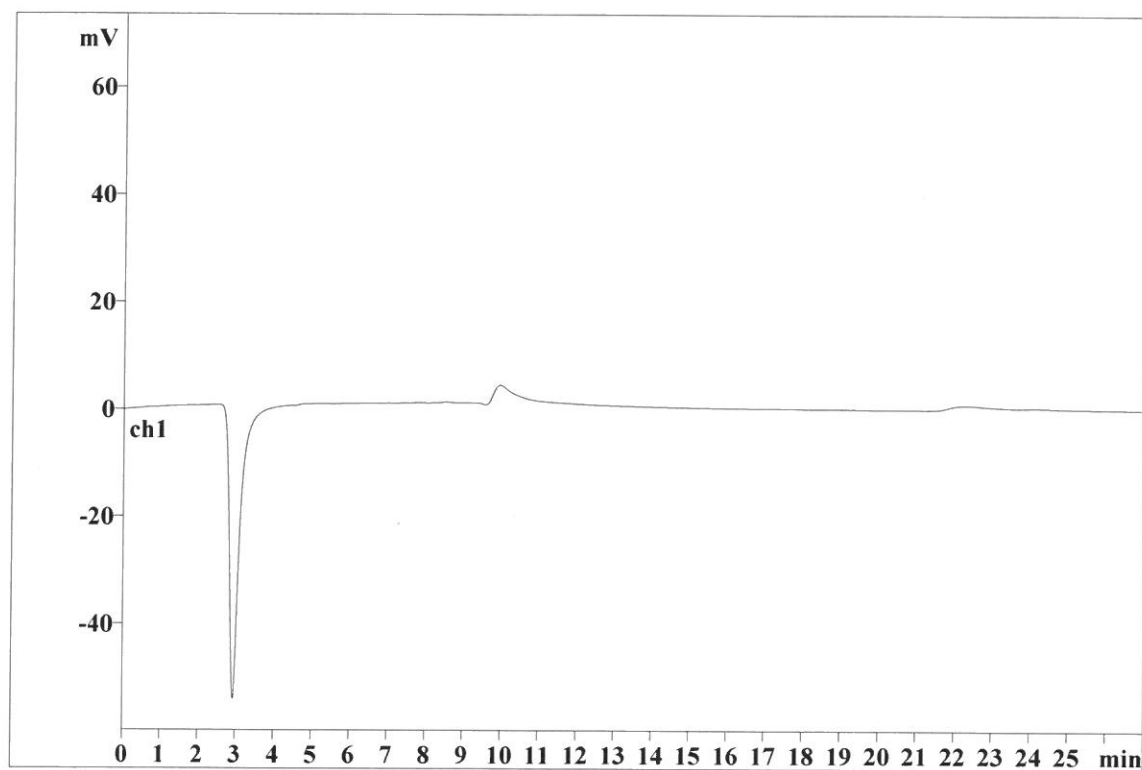

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 11/13/2017 11:33:19 AM
Printed by: wet


Ident: LB91486BSS
Analysis from: 11/7/2017 12:50:45 PM
File: _2017-11-07_

Last save: 11/13/2017 11:32:03 AM

Method: AnionsIC2-110117.mtw
Run operator: wet
Analysis number: 15700

Last save: 11/1/2017 3:19:

SAMPLE: 5.00g
: AK/AP
Vial number: 5
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

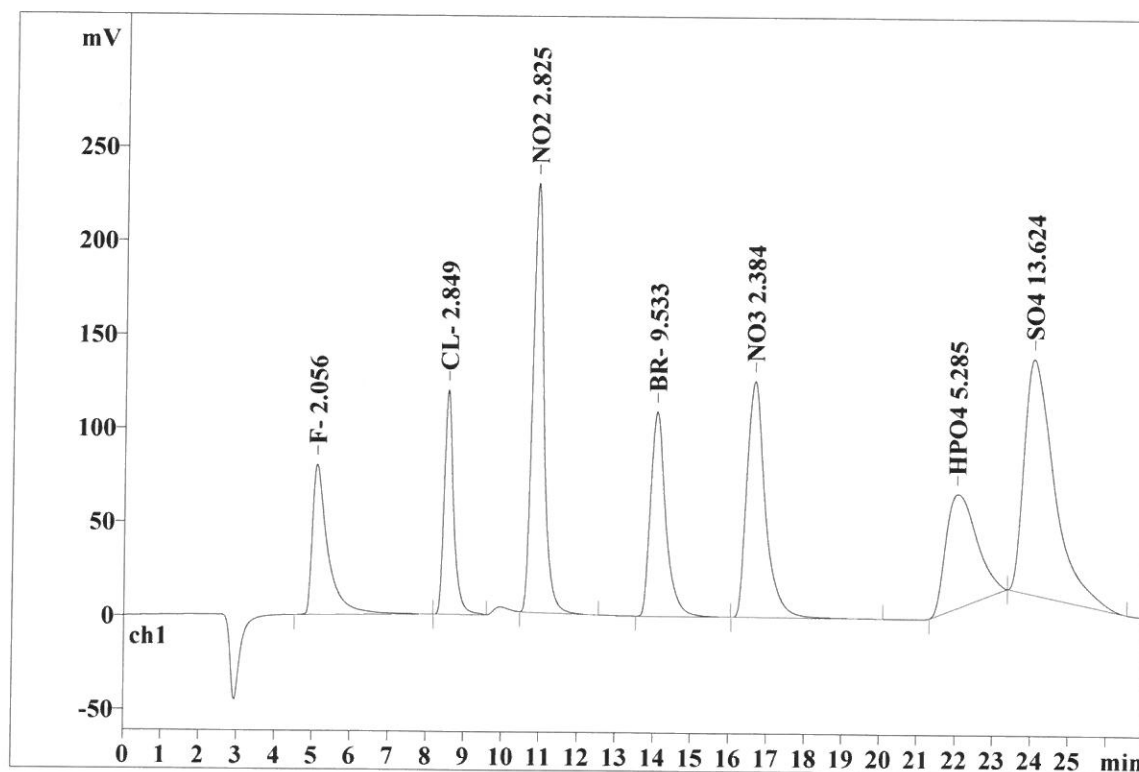

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.09	0.382	80.20	9.43	2309.033	8.55
2	8.54	0.250	119.72	14.08	2078.456	7.70
3	10.88	0.307	228.83	26.92	4761.205	17.64
4	14.06	0.415	109.03	12.83	3079.507	11.41
5	16.63	0.501	125.87	14.81	4288.214	15.88
6	22.01	0.896	60.88	7.16	3445.907	12.76
7	24.03	0.822	125.56	14.77	7034.495	26.06
7	27.00	0.511	850.10	100.00	26996.817	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/13/2017 11:34:55 AM
Printed by: wet


Ident: I6298-01
Analysis from: 11/7/2017 2:11:59 PM
File: _2017-11-07_

Last save: 11/13/2017 11:34:43 AM

Method: AnionsIC2-110117.mtw
Run operator: wet
Analysis number: 15702

Last save: 11/1/2017 3:19:

SAMPLE: 5.01g
: AK/AP
Vial number: 6
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

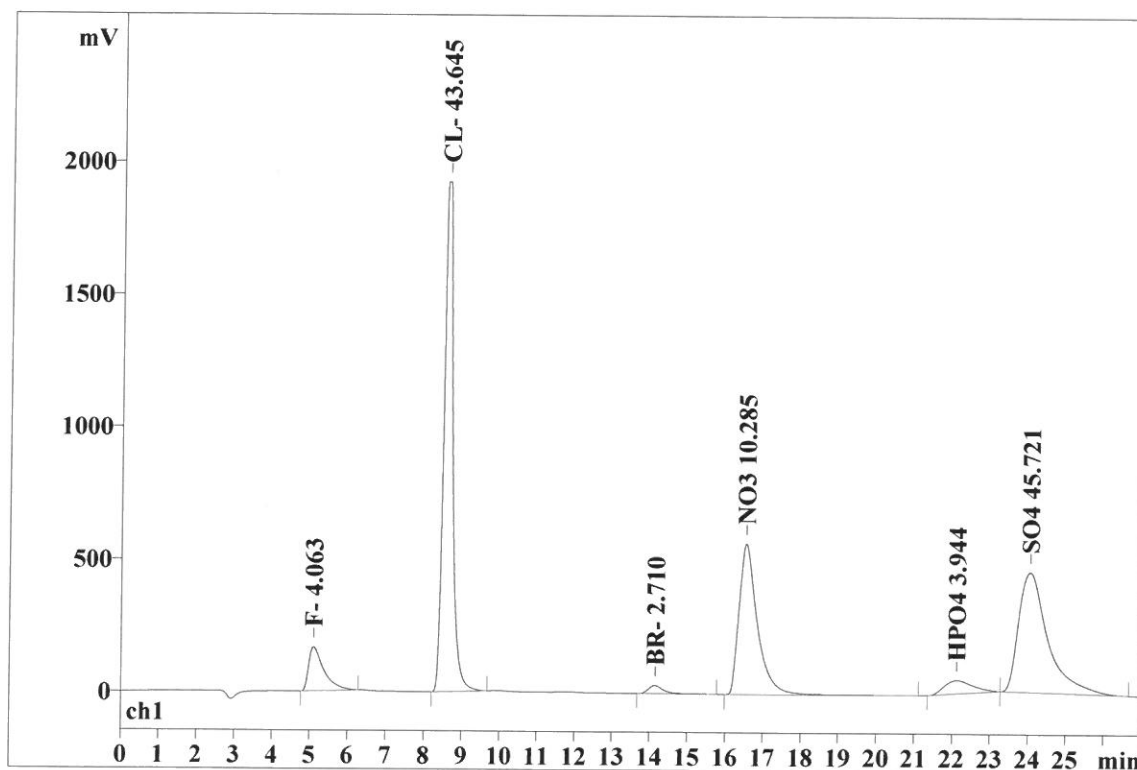

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.10	0.396	165.90	5.20	4596.043	5.46
2	8.61	0.244	1924.97	60.36	32651.618	38.76
3	0.00	0.000	0.00	0.00	0.000	0.00
4	14.15	0.394	30.37	0.95	811.752	0.96
5	16.54	0.486	567.88	17.81	19068.282	22.63
6	22.12	0.835	50.53	1.58	2655.706	3.15
7	24.05	0.768	451.78	14.17	24467.514	29.04
7	27.00	0.446	3191.43	100.08	84250.915	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/13/2017 11:35:17 AM
Printed by: wet


Ident: I6298-01DLX2
Analysis from: 11/7/2017 3:11:55 PM
File: _2017-11-07_

Last save: 11/13/2017 11:35:16 AM

Method: AnionsIC2-110117.mtw
Run operator: wet
Analysis number: 15704

Last save: 11/1/2017 3:19:

SAMPLE: 5.01g
: AK/AP
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

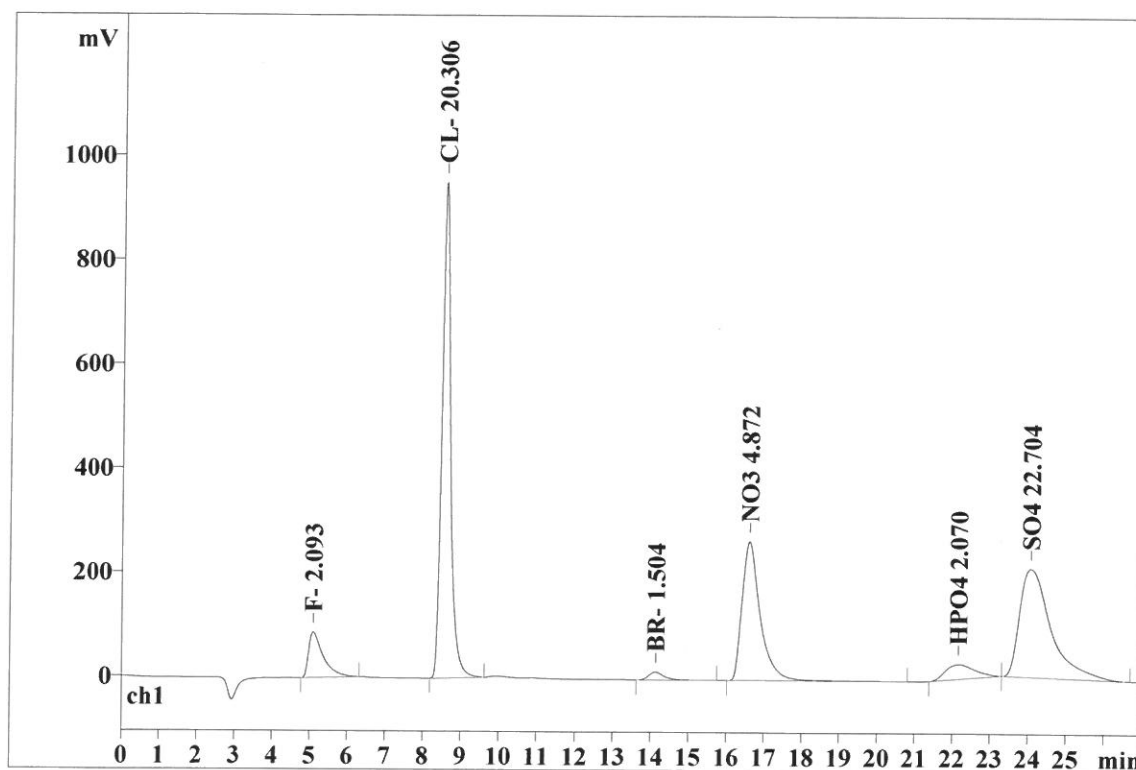

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.09	0.381	87.56	5.62	2350.338	5.82
2	8.55	0.228	952.07	61.13	15161.143	37.54
3	0.00	0.000	0.00	0.00	0.000	0.00
4	14.13	0.405	14.90	0.96	411.058	1.02
5	16.60	0.488	266.68	17.12	8943.131	22.14
6	22.15	0.882	28.24	1.81	1552.530	3.84
7	24.07	0.821	207.90	13.35	11966.445	29.63
7	27.00	0.458	1557.34	100.00	40384.646	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/13/2017 11:35:29 AM
Printed by: wet


Ident: I6298-01DLX10
Analysis from: 11/7/2017 3:41:50 PM
File: _2017-11-07_

Last save: 11/7/2017 4:08:50 PM

Method: AnionsIC2-110117.mtw
Run operator: wet
Analysis number: 15705

Last save: 11/1/2017 3:19:

SAMPLE: 5.01g
: AK/AP
Vial number: 12
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

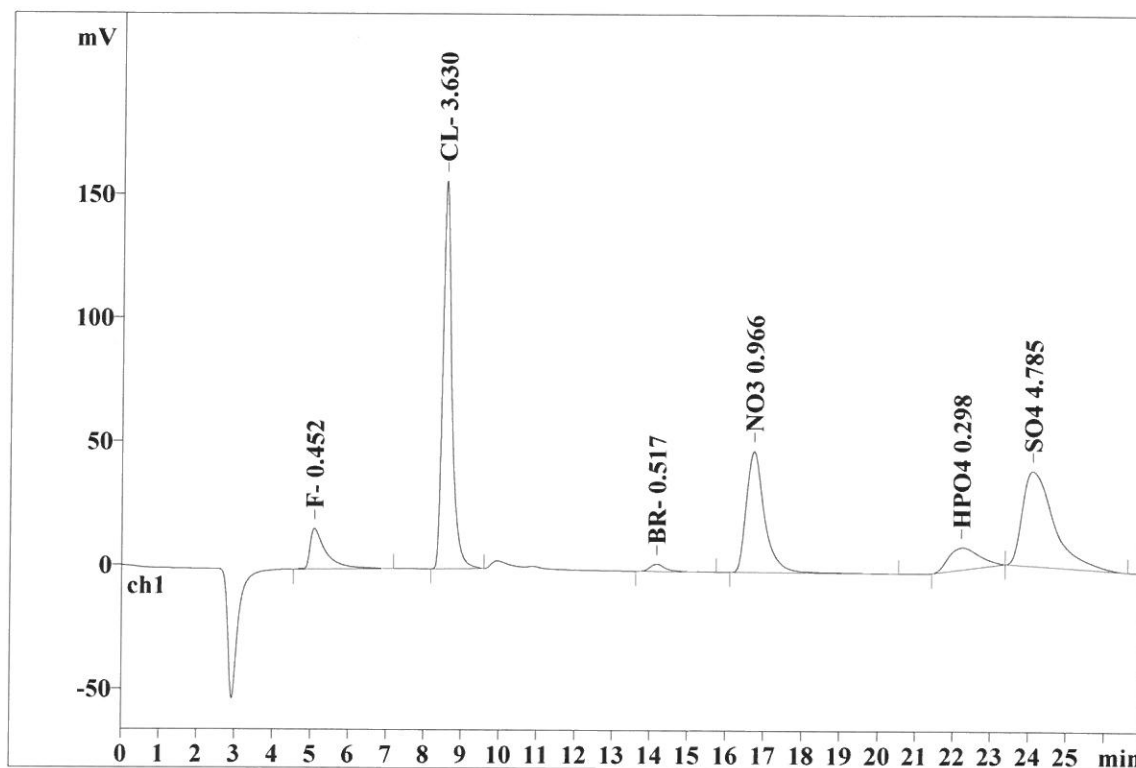

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.08	0.382	16.47	6.04	481.104	6.33
2	8.55	0.244	156.84	57.56	2663.507	35.02
3	0.00	0.000	0.00	0.00	0.000	0.00
4	14.17	0.412	2.95	1.08	83.090	1.09
5	16.72	0.485	48.90	17.95	1635.274	21.50
6	22.21	0.919	8.94	3.28	508.747	6.69
7	24.10	0.840	38.35	14.08	2233.581	29.37
7	27.00	0.469	272.46	100.00	7605.302	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/13/2017 11:35:34 AM
Printed by: wet


Ident: CCV
Analysis from: 11/7/2017 4:11:52 PM
File: _2017-11-07_

Last save: 11/7/2017 4:38:52 PM

Method: AnionsIC2-110117.mtw
Run operator: wet
Analysis number: 15706

Last save: 11/1/2017 3:19:

SAMPLE:
: AK/AP
Vial number: 2
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

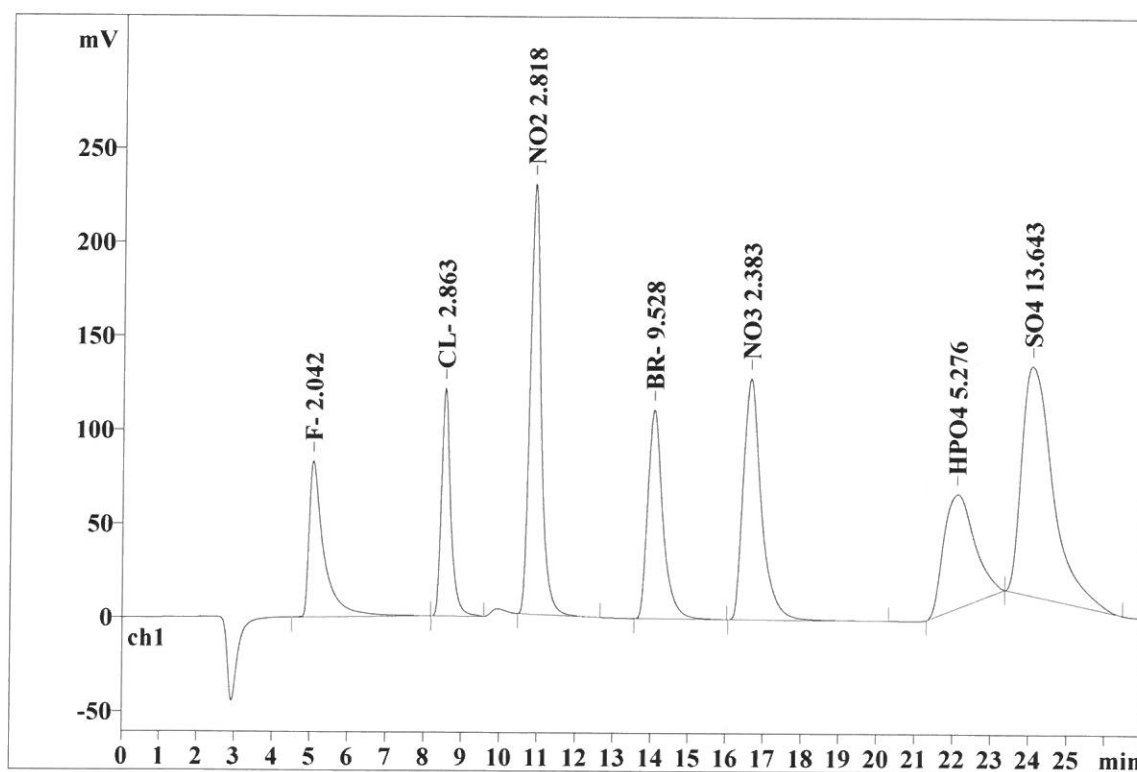

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.07	0.356	83.04	9.69	2292.862	8.50
2	8.54	0.246	121.45	14.18	2088.709	7.74
3	10.89	0.304	229.38	26.77	4750.142	17.61
4	14.06	0.406	111.19	12.98	3078.024	11.41
5	16.64	0.488	128.46	14.99	4285.636	15.88
6	22.09	0.892	60.89	7.11	3440.115	12.75
7	24.06	0.840	122.36	14.28	7044.966	26.11
7	27.00	0.505	856.76	100.00	26980.454	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/13/2017 11:35:41 AM
Printed by: wet


Ident: CCB
Analysis from: 11/7/2017 4:45:14 PM
File: _2017-11-07_

Last save: 11/13/2017 11:32:51 AM

Method: AnionsIC2-110117.mtw
Run operator: wet
Analysis number: 15707

Last save: 11/1/2017 3:19:

SAMPLE:
: AK/AP
Vial number: 3
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

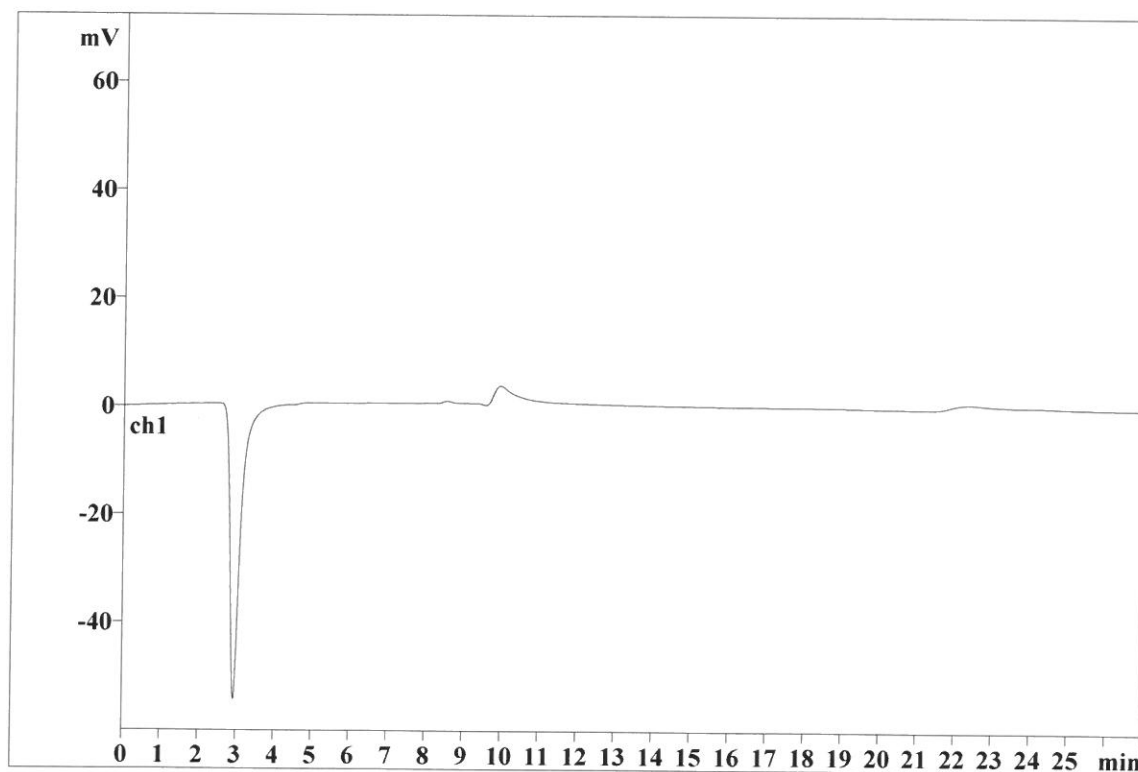

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD