


245.1

LB 91516
INSTRUMENT ID: CV1

Linear

 μ Abs.:

32151

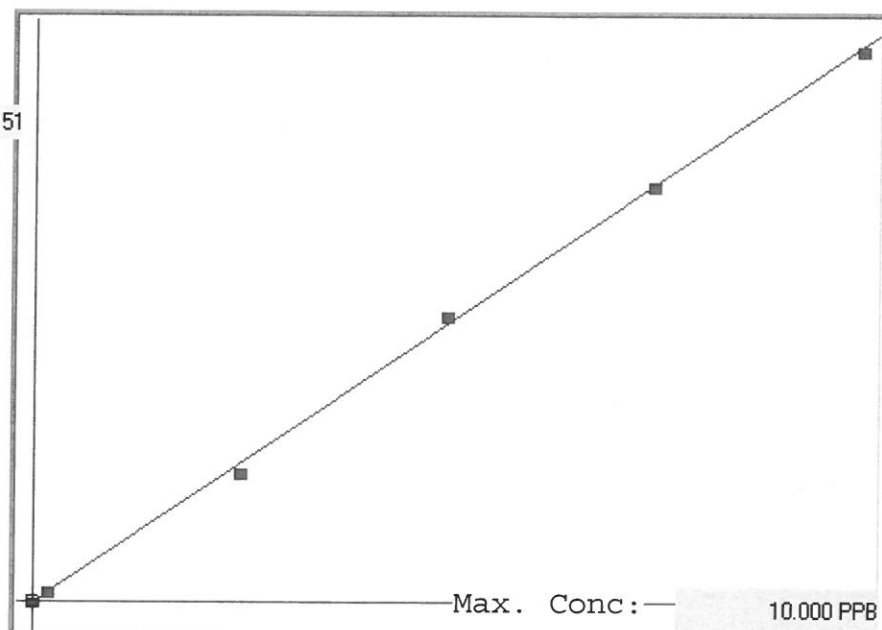

A= 0.0000e+000

B= 3.0851e-004

C= 2.3971e-002

Rho= 0.9996694

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.006	0.006	-59	0.000	-59				
0.2	0.200	0.222	0.022	642	0.0 %	642				
2.5	2.500	2.356	-0.144	7558	0.0 %	7558				
5.0	5.000	5.171	0.171	16685	0.0 %	16685				
7.5	7.500	7.502	0.002	24241	0.0 %	24241				
10.0	10.000	9.943	-0.057	32151	0.0 %	32151				

LB91516 INSTRUMENT ID : CV1

Method: 245.1

Operator: Admin

Date of Analysis: 10 Nov 2017 14:59:24

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-59	-	0.0000	245.1	PPB	10 Nov 2017 15:14:08	S	Std
0.2 - 1	50.2	642	-	0.2000	245.1	PPB	10 Nov 2017 15:16:16	S	Std
2.5 - 1	52.5	7558	-	2.5000	245.1	PPB	10 Nov 2017 15:18:25	S	Std
5.0 - 1	55	16685	-	5.0000	245.1	PPB	10 Nov 2017 15:20:33	S	Std
7.5 - 1	57.5	24241	-	7.5000	245.1	PPB	10 Nov 2017 15:22:41	S	Std
10.0 - 1	510	32151	-	10.0000	245.1	PPB	10 Nov 2017 15:24:49	S	Std
ICV58 - 1	ICV58	12401	3.8497	-245.1		PPB	10 Nov 2017 15:27:26	U	SMPL
ICB58 - 1	ICB58	-145	-0.0208	-245.1		PPB	10 Nov 2017 15:29:33	U	SMPL
CCV60 - 1	CCV60	16781	5.2010	-245.1		PPB	10 Nov 2017 15:31:40	U	SMPL
CCB60 - 1	CCB60	-163	-0.0263	-245.1		PPB	10 Nov 2017 15:33:47	U	SMPL
CRA - 1	CRA	637	0.2205	-245.1		PPB	10 Nov 2017 15:35:54	U	SMPL
HighStd - 1	HighStd	32362	10.0078	-245.1		PPB	10 Nov 2017 15:38:01	U	SMPL
ChkStd - 1	ChkStd	20896	6.4705	-245.1		PPB	10 Nov 2017 15:40:07	U	SMPL
PB104144BL - 1	PBW	227	0.0940	-245.1		PPB	10 Nov 2017 15:42:16	U	SMPL
PB104144BS - 1	LCSW	13095	4.0638	-245.1		PPB	10 Nov 2017 15:44:25	U	SMPL
I6402-01 - 1	110717-TIDO-F-D-B	131	0.0644	-245.1		PPB	10 Nov 2017 15:46:33	U	SMPL
I6402-02 - 1	110717-TIDO-F-D-S	169	0.0761	-245.1		PPB	10 Nov 2017 15:48:41	U	SMPL
I6402-03 - 1	110717-TIDO-F-U-B	126	0.0628	-245.1		PPB	10 Nov 2017 15:50:49	U	SMPL
I6402-04 - 1	110717-TIDO-F-U-S	122	0.0616	-245.1		PPB	10 Nov 2017 15:52:58	U	SMPL
I6402-05 - 1	110717-SIDI-F-D-B	165	0.0749	-245.1		PPB	10 Nov 2017 15:55:04	U	SMPL
CCV61 - 1	CCV61	16764	5.1958	-245.1		PPB	10 Nov 2017 15:57:11	U	SMPL
CCB61 - 1	CCB61	-163	-0.0263	-245.1		PPB	10 Nov 2017 15:59:18	U	SMPL
I6402-06 - 1	110717-SIDI-F-D-S	146	0.0690	-245.1		PPB	10 Nov 2017 16:01:26	U	SMPL
I6402-07 - 1	110717-SIDI-F-U-B	155	0.0718	-245.1		PPB	10 Nov 2017 16:03:33	U	SMPL
I6402-08 - 1	110717-SIDI-F-U-S	127	0.0632	-245.1		PPB	10 Nov 2017 16:05:39	U	SMPL
I6402-09 - 1	110717-JETT-E-D-B	130	0.0641	-245.1		PPB	10 Nov 2017 16:07:46	U	SMPL
I6402-10 - 1	110717-JETT-E-D-S	121	0.0613	-245.1		PPB	10 Nov 2017 16:09:54	U	SMPL
I6402-11 - 1	110717-JETT-E-U-B	105	0.0564	-245.1		PPB	10 Nov 2017 16:12:01	U	SMPL
I6402-12 - 1	110717-JETT-E-U-S	82	0.0493	-245.1		PPB	10 Nov 2017 16:14:09	U	SMPL
I6402-12DUP - 1	110717-JETT-E-U-SDUP	87	0.0508	-245.1		PPB	10 Nov 2017 16:16:17	U	SMPL
I6402-12MS - 1	110717-JETT-E-U-SMS	14723	4.5661	-245.1		PPB	10 Nov 2017 16:18:26	U	SMPL
I6402-12MSD - 1	110717-JETT-E-U-SMSD	14582	4.5226	-245.1		PPB	10 Nov 2017 16:20:33	U	SMPL
CCV62 - 1	CCV62	16585	5.1405	-245.1		PPB	10 Nov 2017 16:22:40	U	SMPL
CCB62 - 1	CCB62	-155	-0.0238	-245.1		PPB	10 Nov 2017 16:24:47	U	SMPL
PB104145BL - 1	PBW	172	0.0770	-245.1		PPB	10 Nov 2017 16:34:35	U	SMPL
PB104145BS - 1	LCSW	13199	4.0959	-245.1		PPB	10 Nov 2017 16:36:42	U	SMPL
I6403-01 - 1	110817-JETT-F-D-B	29	0.0329	-245.1		PPB	10 Nov 2017 16:38:49	U	SMPL
I6403-02 - 1	110817-JETT-F-D-S	79	0.0483	-245.1		PPB	10 Nov 2017 16:40:56	U	SMPL
I6403-03 - 1	110817-JETT-F-U-B	78	0.0480	-245.1		PPB	10 Nov 2017 16:43:03	U	SMPL
I6403-04 - 1	110817-JETT-F-U-S	74	0.0468	-245.1		PPB	10 Nov 2017 16:45:11	U	SMPL
I6403-05 - 1	110817-TIDO-F-D-B	75	0.0471	-245.1		PPB	10 Nov 2017 16:51:46	U	SMPL
I6403-06 - 1	110817-TIDO-F-D-S	94	0.0530	-245.1		PPB	10 Nov 2017 16:53:54	U	SMPL
I6403-07 - 1	110817-TIDO-F-U-B	100	0.0548	-245.1		PPB	10 Nov 2017 16:56:03	U	SMPL
I6403-08 - 1	110817-TIDO-F-U-S	88	0.0511	-245.1		PPB	10 Nov 2017 16:58:10	U	SMPL
CCV63 - 1	CCV63	16517	5.1196	-245.1		PPB	10 Nov 2017 17:00:17	U	SMPL
CCB63 - 1	CCB63	-164	-0.0266	-245.1		PPB	10 Nov 2017 17:02:24	U	SMPL
I6403-09 - 1	110817-SIDI-F-D-B	71	0.0459	-245.1		PPB	10 Nov 2017 17:04:33	U	SMPL
I6403-10 - 1	110817-SIDI-F-D-M	77	0.0477	-245.1		PPB	10 Nov 2017 17:06:40	U	SMPL
I6403-11 - 1	110817-SIDI-F-D-S	83	0.0496	-245.1		PPB	10 Nov 2017 17:08:47	U	SMPL
I6403-12 - 1	110817-SIDI-F-U-B	97	0.0539	-245.1		PPB	10 Nov 2017 17:10:55	U	SMPL
I6403-13 - 1	110817-SIDI-F-U-M	104	0.0561	-245.1		PPB	10 Nov 2017 17:13:02	U	SMPL
I6403-14 - 1	110817-SIDI-F-U-S	85	0.0502	-245.1		PPB	10 Nov 2017 17:15:09	U	SMPL
I6403-14DUP - 1	110817-SIDI-F-U-SDUP	96	0.0536	-245.1		PPB	10 Nov 2017 17:17:17	U	SMPL
I6403-14MS - 1	110817-SIDI-F-U-SMS	14811	4.5932	-245.1		PPB	10 Nov 2017 17:19:26	U	SMPL
I6403-14MSD - 1	110817-SIDI-F-U-SMSD	14801	4.5902	-245.1		PPB	10 Nov 2017 17:21:34	U	SMPL
CCV64 - 1	CCV64	16453	5.0998	-245.1		PPB	10 Nov 2017 17:31:35	U	SMPL
CCB64 - 1	CCB64	-163	-0.0263	-245.1		PPB	10 Nov 2017 17:33:42	U	SMPL
I6402-12LX5 - 1		-6	0.0221	-245.1		PPB	10 Nov 2017 17:37:42	U	SMPL
I6402-12A - 1		14362	4.4547	-245.1		PPB	10 Nov 2017 17:39:49	U	SMPL
I6403-14LX5 - 1		-83	-0.0016	-245.1		PPB	10 Nov 2017 17:41:56	U	SMPL
I6403-14A - 1		14860	4.6084	-245.1		PPB	10 Nov 2017 17:44:04	U	SMPL
CCV65 - 1	CCV65	16148	5.0057	-245.1		PPB	10 Nov 2017 17:46:11	U	SMPL
CCB65 - 1	CCB65	-178	-0.0309	-245.1		PPB	10 Nov 2017 17:48:19	U	SMPL