


LB 91612

ISM02.4

 μ Abs.:

4088E

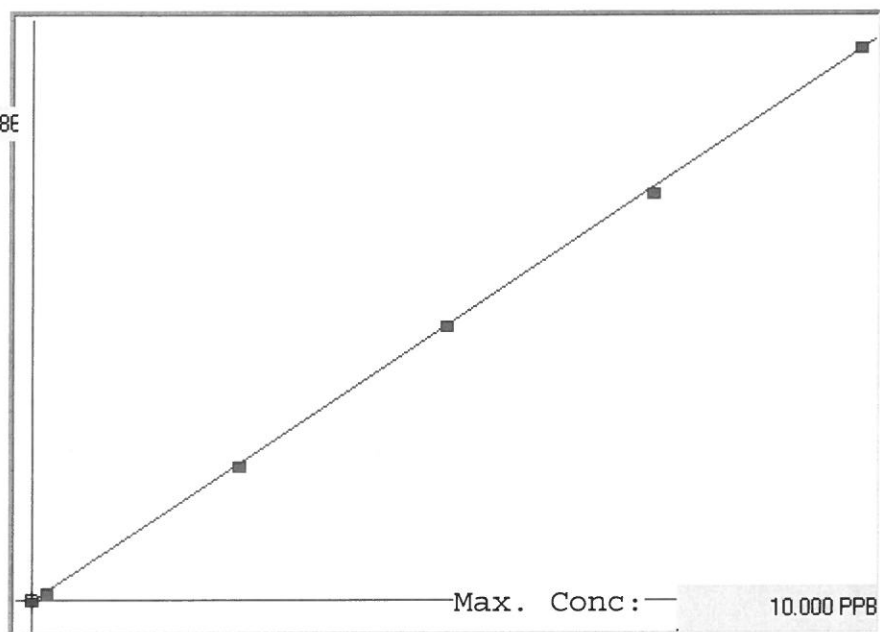

Linear

A= 0.0000e+000

B= 2.4452e-004

C= 4.4743e-002

Rho= 0.9999612

Accept=Accepted

slope
intercept

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	g/d
0.00	0.000	0.011	0.011	-138	0.000	-138					1
0.2	0.200	0.205	0.005	656	0.0 %	656					2
2.5	2.500	2.491	-0.009	10004	0.0 %	10004					0
5.0	5.000	5.015	0.015	20326	0.0 %	20326					0
7.5	7.500	7.436	-0.064	30227	0.0 %	30227					1
10.0	10.000	10.042	0.042	40886	0.0 %	40886					0

NB
11/17/18

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type
	0 S0.0	-138	-		0 ISM02.4	PPB	11/15/2017 14:44	Std
	0.2 S0.2	656	-		0.2 ISM02.4	PPB	11/15/2017 14:48	Std
	2.5 S2.5	10004	-		2.5 ISM02.4	PPB	11/15/2017 14:51	Std
	5 S5	20326	-		5 ISM02.4	PPB	11/15/2017 14:53	Std
	7.5 S7.5	30227	-		7.5 ISM02.4	PPB	11/15/2017 14:55	Std
	10 S10	40886	-		10 ISM02.4	PPB	11/15/2017 14:58	Std
ICV	ICV	15937	3.9417 -		ISM02.4	PPB	11/15/2017 15:00	SMPL
ICB	ICB	-289	-0.0259 -		ISM02.4	PPB	11/15/2017 15:03	SMPL
CCV013	CCV013	20219	4.9887 -		ISM02.4	PPB	11/15/2017 15:05	SMPL
CCB013	CCB013	-290	-0.0262 -		ISM02.4	PPB	11/15/2017 15:07	SMPL
PB104276BL	PBW003	80	0.0643 -		ISM02.4	PPB	11/15/2017 15:09	SMPL
I6406-01	MBE2S7	401	0.1428 -		ISM02.4	PPB	11/15/2017 15:12	SMPL
I6406-02	MBE2S8	198	0.0932 -		ISM02.4	PPB	11/15/2017 15:14	SMPL
I6406-03	MBE2S9	106	0.0707 -		ISM02.4	PPB	11/15/2017 15:16	SMPL
I6406-04	MBE2T0	107	0.0709 -		ISM02.4	PPB	11/15/2017 15:19	SMPL
I6406-05	MBE2T1	68	0.0614 -		ISM02.4	PPB	11/15/2017 15:21	SMPL
I6406-06	MBE2T3	324	0.124 -		ISM02.4	PPB	11/15/2017 15:23	SMPL
I6406-07	MBE2T4	111	0.0719 -		ISM02.4	PPB	11/15/2017 15:25	SMPL
I6406-08	MBE2T5	93	0.0675 -		ISM02.4	PPB	11/15/2017 15:28	SMPL
I6406-09	MBE2T6	106	0.0707 -		ISM02.4	PPB	11/15/2017 15:30	SMPL
I6406-10	MBE2T7	68	0.0614 -		ISM02.4	PPB	11/15/2017 15:32	SMPL
I6406-11	MBE2T8	98	0.0687 -		ISM02.4	PPB	11/15/2017 15:35	SMPL
I6406-12	MBE2T9	71	0.0621 -		ISM02.4	PPB	11/15/2017 15:37	SMPL
I6406-13	MBE2W0	71	0.0621 -		ISM02.4	PPB	11/15/2017 15:39	SMPL
I6406-14	MBE2W0D	56	0.0584 -		ISM02.4	PPB	11/15/2017 15:41	SMPL
I6406-15	MBE2W0S	3654	0.9382 -		ISM02.4	PPB	11/15/2017 15:44	SMPL
I6406-16	MBE2W1	68	0.0614 -		ISM02.4	PPB	11/15/2017 15:46	SMPL
I6406-17	MBE2W2	93	0.0675 -		ISM02.4	PPB	11/15/2017 15:48	SMPL
I6406-18	MBE2W3	95	0.068 -		ISM02.4	PPB	11/15/2017 15:50	SMPL
I6406-19	MBE2W4	83	0.065 -		ISM02.4	PPB	11/15/2017 15:53	SMPL
CCV014	CCV014	20245	4.9951 -		ISM02.4	PPB	11/15/2017 15:55	SMPL
CCB014	CCB014	-282	-0.0242 -		ISM02.4	PPB	11/15/2017 15:57	SMPL
I6406-20	MBE2W6	93	0.0675 -		ISM02.4	PPB	11/15/2017 16:00	SMPL
I6406-21	MBE2W7	44	0.0555 -		ISM02.4	PPB	11/15/2017 16:02	SMPL
I6406-22	MBE2W8	39	0.0543 -		ISM02.4	PPB	11/15/2017 16:04	SMPL
PB104277BL	PBW003	78	0.0638 -		ISM02.4	PPB	11/15/2017 16:06	SMPL
I6457-01	METO23	478	0.1616 -		ISM02.4	PPB	11/15/2017 16:09	SMPL
I6457-02	METO26	-139	0.0108 -		ISM02.4	PPB	11/15/2017 16:11	SMPL
I6457-03	METO26D	-168	0.0037 -		ISM02.4	PPB	11/15/2017 16:13	SMPL
I6457-04	METO26S	4111	1.05 -		ISM02.4	PPB	11/15/2017 16:15	SMPL
I6457-05	METO30	-237	-0.0132 -		ISM02.4	PPB	11/15/2017 16:18	SMPL
I6457-06	METO32	-196	-0.0032 -		ISM02.4	PPB	11/15/2017 16:20	SMPL
I6457-07	METO36	-194	-0.0027 -		ISM02.4	PPB	11/15/2017 16:22	SMPL
I6457-09	METO50	-203	-0.0049 -		ISM02.4	PPB	11/15/2017 16:25	SMPL
I6457-10	METO66	-218	-0.0086 -		ISM02.4	PPB	11/15/2017 16:27	SMPL
I6457-11	METO38	-183	0 -		ISM02.4	PPB	11/15/2017 16:29	SMPL

INSTRUMENT ID : CV1

I6457-12	METO48	-186	-0.0007 -	ISM02.4	PPB	11/15/2017 16:31 SMPL
I6457-13	METO52	-199	-0.0039 -	ISM02.4	PPB	11/15/2017 16:34 SMPL
I6457-14	METO54	-211	-0.0069 -	ISM02.4	PPB	11/15/2017 16:36 SMPL
I6457-15	METO56	-199	-0.0039 -	ISM02.4	PPB	11/15/2017 16:38 SMPL
I6457-16	METO60	-159	0.0059 -	ISM02.4	PPB	11/15/2017 16:41 SMPL
I6457-17	METO70	-156	0.0066 -	ISM02.4	PPB	11/15/2017 16:43 SMPL
CCV015	CCV015	20291	5.0063 -	ISM02.4	PPB	11/15/2017 16:45 SMPL
CCB015	CCB015	-278	-0.0232 -	ISM02.4	PPB	11/15/2017 16:47 SMPL
I6457-18	METO72	87	0.066 -	ISM02.4	PPB	11/15/2017 16:50 SMPL
PB104278BL	PBW003	29	0.0518 -	ISM02.4	PPB	11/15/2017 16:52 SMPL
I6458-01	METO24	31	0.0523 -	ISM02.4	PPB	11/15/2017 16:54 SMPL
I6458-02	METO27	33	0.0528 -	ISM02.4	PPB	11/15/2017 16:57 SMPL
I6458-03	METO27D	26	0.0511 -	ISM02.4	PPB	11/15/2017 16:59 SMPL
I6458-04	METO27S	4001	1.0231 -	ISM02.4	PPB	11/15/2017 17:01 SMPL
I6458-05	METO31	-81	0.0249 -	ISM02.4	PPB	11/15/2017 17:03 SMPL
I6458-06	METO33	-54	0.0315 -	ISM02.4	PPB	11/15/2017 17:06 SMPL
I6458-07	METO37	-57	0.0308 -	ISM02.4	PPB	11/15/2017 17:08 SMPL
I6458-09	METO51	-24	0.0389 -	ISM02.4	PPB	11/15/2017 17:10 SMPL
I6458-10	METO67	-18	0.0403 -	ISM02.4	PPB	11/15/2017 17:12 SMPL
I6458-11	METO39	-32	0.0369 -	ISM02.4	PPB	11/15/2017 17:15 SMPL
I6458-12	METO49	-20	0.0399 -	ISM02.4	PPB	11/15/2017 17:17 SMPL
I6458-13	METO53	-24	0.0389 -	ISM02.4	PPB	11/15/2017 17:19 SMPL
I6458-14	METO55	-37	0.0357 -	ISM02.4	PPB	11/15/2017 17:22 SMPL
I6458-15	METO57	-31	0.0372 -	ISM02.4	PPB	11/15/2017 17:24 SMPL
I6458-16	METO61	-7	0.043 -	ISM02.4	PPB	11/15/2017 17:26 SMPL
I6458-17	METO71	-9	0.0425 -	ISM02.4	PPB	11/15/2017 17:28 SMPL
I6458-18	METO73	-10	0.0423 -	ISM02.4	PPB	11/15/2017 17:31 SMPL
CCV016	CCV016	20022	4.9405 -	ISM02.4	PPB	11/15/2017 17:33 SMPL
CCB016	CCB016	-313	-0.0318 -	ISM02.4	PPB	11/15/2017 17:35 SMPL