


7470A

LB 91833
INSTRUMENT ID: CV2

Linear

 μ Abs.:

35872

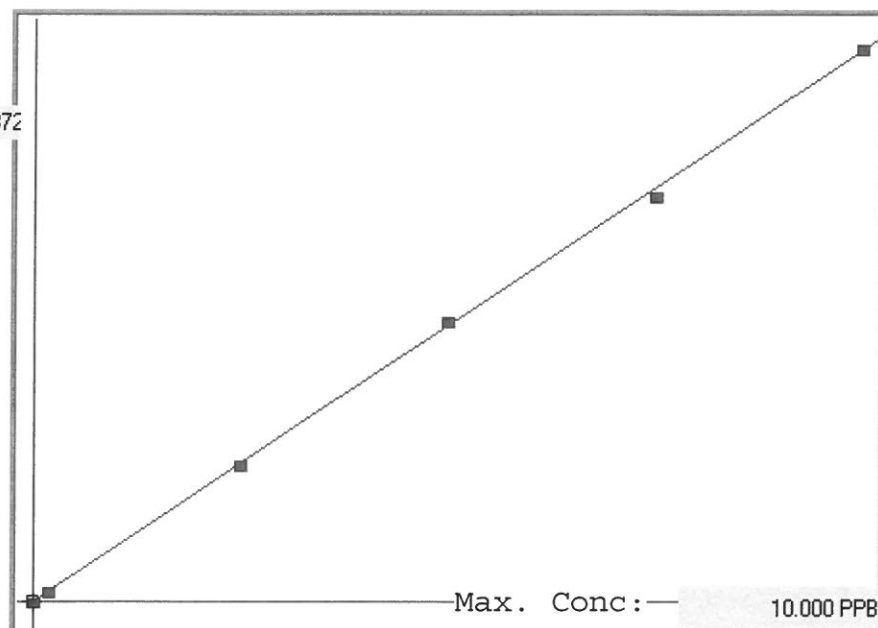

A= 0.0000e+000

B= 2.7993e-004

C= 3.8181e-003

Rho= 0.9998445

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.010	-0.010	-51	0.000	-51				
0.2	0.200	0.201	0.001	706	0.0 %	706				
2.5	2.500	2.496	-0.004	8904	0.0 %	8904				
5.0	5.000	5.090	0.090	18170	0.0 %	18170				
7.5	7.500	7.377	-0.123	26340	0.0 %	26340				
10.0	10.000	10.045	0.045	35872	0.0 %	35872				

LB91833 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 29 Nov 2017 09:48:56

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-51	-	0.0000	7470A	PPB	29 Nov 2017 10:00:28	S	Std
0.2 - 1	50.2	706	-	0.2000	7470A	PPB	29 Nov 2017 10:02:37	S	Std
2.5 - 1	52.5	8904	-	2.5000	7470A	PPB	29 Nov 2017 10:04:45	S	Std
5.0 - 1	55	18170	-	5.0000	7470A	PPB	29 Nov 2017 10:06:54	S	Std
7.5 - 1	57.5	26340	-	7.5000	7470A	PPB	29 Nov 2017 10:09:02	S	Std
10.0 - 1	510	35872	-	10.0000	7470A	PPB	29 Nov 2017 10:13:34	S	Std
ICV82 - 1	ICV82	13838	3.8775	-7470A	PPB	PPB	29 Nov 2017 10:16:05	U	SMPL
ICB82 - 1	ICB82	-183	-0.0474	-7470A	PPB	PPB	29 Nov 2017 10:18:11	U	SMPL
CCV11 - 1	CCV11	18336	5.1366	-7470A	PPB	PPB	29 Nov 2017 10:20:18	U	SMPL
CCB11 - 1	CCB11	-179	-0.0463	-7470A	PPB	PPB	29 Nov 2017 10:22:24	U	SMPL
CRA - 1	CRA	693	0.1978	-7470A	PPB	PPB	29 Nov 2017 10:24:32	U	SMPL
HighStd - 1	HighStd	36004	10.0824	-7470A	PPB	PPB	29 Nov 2017 10:26:38	U	SMPL
ChkStd - 1	ChkStd	25389	7.1109	-7470A	PPB	PPB	29 Nov 2017 10:28:45	U	SMPL
PB104584BL - 1	PBW	-245	-0.0648	-7470A	PPB	PPB	29 Nov 2017 10:30:54	U	SMPL
PB104584BS - 1	LCSW	13376	3.7481	-7470A	PPB	PPB	29 Nov 2017 10:33:03	U	SMPL
PB104584TB - 1	PB104558TB	-133	-0.0334	-7470A	PPB	PPB	29 Nov 2017 10:35:10	U	SMPL
I6601-01 - 1	CONCRETE-DEBRIS	53	0.0187	-7470A	PPB	PPB	29 Nov 2017 10:37:18	U	SMPL
I6601-01DUP - 1	CONCRETE-DEBRISDUP	62	0.0212	-7470A	PPB	PPB	29 Nov 2017 10:39:26	U	SMPL
I6601-01MS - 1	CONCRETE-DEBRISMS	12860	3.6037	-7470A	PPB	PPB	29 Nov 2017 10:41:34	U	SMPL
I6601-01MSD - 1	CONCRETE-DEBRISMSD	13103	3.6717	-7470A	PPB	PPB	29 Nov 2017 10:43:41	U	SMPL
CCV12 - 1	CCV12	18356	5.1422	-7470A	PPB	PPB	29 Nov 2017 10:45:48	U	SMPL
CCB12 - 1	CCB12	-172	-0.0443	-7470A	PPB	PPB	29 Nov 2017 10:47:55	U	SMPL
I6602-03 - 1	ETGI-294	-45	-0.0088	-7470A	PPB	PPB	29 Nov 2017 10:50:02	U	SMPL
I6601-01LX5 - 1		-13	0.0002	-7470A	PPB	PPB	29 Nov 2017 10:52:09	U	SMPL
I6601-01A - 1		13719	3.8442	-7470A	PPB	PPB	29 Nov 2017 10:54:16	U	SMPL
CCV13 - 1	CCV13	18071	5.0624	-7470A	PPB	PPB	29 Nov 2017 10:56:23	U	SMPL
CCB13 - 1	CCB13	-168	-0.0432	-7470A	PPB	PPB	29 Nov 2017 10:58:31	U	SMPL