

7470A


LB 91936

INSTRUMENT ID: CV1

Linear

 μ Abs.:

34605

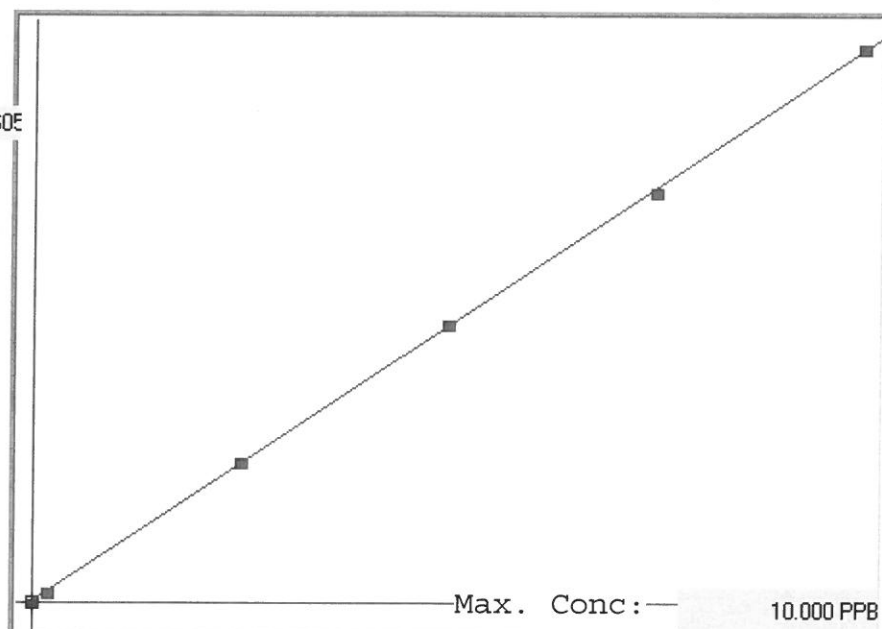

A= 0.0000e+000

B= 2.9019e-004

C= -1.4879e-002

Rho= 0.9999547

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.007	-0.007	28	0.000	28				
0.2	0.200	0.186	-0.014	691	0.0 %	691				
2.5	2.500	2.531	0.031	8774	0.0 %	8774				
5.0	5.000	5.030	0.030	17384	0.0 %	17384				
7.5	7.500	7.433	-0.067	25664	0.0 %	25664				
10.0	10.000	10.027	0.027	34605	0.0 %	34605				

LB91936 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 05 Dec 2017 10:04:05

Sample ID	Extended ID	μ Abs	Conc.	Std Cond	Method	Units	Date	Type	Type
0.0 - 1	50	28	-	0.0000	7470A	PPB	05 Dec 2017 10:08:41	S	Std
0.2 - 1	50.2	691	-	0.2000	7470A	PPB	05 Dec 2017 10:10:49	S	Std
2.5 - 1	52.5	8774	-	2.5000	7470A	PPB	05 Dec 2017 10:12:58	S	Std
5.0 - 1	55	17384	-	5.0000	7470A	PPB	05 Dec 2017 10:15:06	S	Std
7.5 - 1	57.5	25664	-	7.5000	7470A	PPB	05 Dec 2017 10:17:14	S	Std
10.0 - 1	51.0	34605	-	10.0000	7470A	PPB	05 Dec 2017 10:19:23	S	Std
ICV89 - 1	ICV89	13370	3.8650	-	7470A	PPB	05 Dec 2017 10:22:02	U	SMPL
ICB89 - 1	ICB89	-106	-0.0456	-	7470A	PPB	05 Dec 2017 10:24:08	U	SMPL
CCV44 - 1	CCV44	17352	5.0206	-	7470A	PPB	05 Dec 2017 10:26:15	U	SMPL
CCB44 - 1	CCB44	-106	-0.0456	-	7470A	PPB	05 Dec 2017 10:28:22	U	SMPL
CRA - 1	CRA	674	0.1807	-	7470A	PPB	05 Dec 2017 10:30:29	U	SMPL
HighStd - 1	HighStd	34929	10.1213	-	7470A	PPB	05 Dec 2017 10:32:36	U	SMPL
ChkStd - 1	ChkStd	24627	7.1317	-	7470A	PPB	05 Dec 2017 10:34:43	U	SMPL
PB104693BL - 1	PBW	-205	-0.0744	-	7470A	PPB	05 Dec 2017 10:36:52	U	SMPL
PB104693BS - 1	LCSW	14140	4.0885	-	7470A	PPB	05 Dec 2017 10:39:01	U	SMPL
PB104693TB - 1	PB104637TB	-112	-0.0474	-	7470A	PPB	05 Dec 2017 10:41:09	U	SMPL
I6308-02 - 1	SA-06-120117	-21	-0.0210	-	7470A	PPB	05 Dec 2017 10:43:16	U	SMPL
I6308-02DUP - 1	SA-06-120117DUP	-11	-0.0181	-	7470A	PPB	05 Dec 2017 10:45:25	U	SMPL
I6308-02MS - 1	SA-06-120117MS	13756	3.9770	-	7470A	PPB	05 Dec 2017 10:47:34	U	SMPL
I6308-02MSD - 1	SA-06-120117MSD	13045	3.7707	-	7470A	PPB	05 Dec 2017 10:49:40	U	SMPL
CCV45 - 1	CCV45	17440	5.0461	-	7470A	PPB	05 Dec 2017 10:51:47	U	SMPL
CCB45 - 1	CCB45	-102	-0.0445	-	7470A	PPB	05 Dec 2017 10:53:53	U	SMPL
I6659-04 - 1	TRANSFORMER-1-2	8	-0.0126	-	7470A	PPB	05 Dec 2017 10:56:01	U	SMPL
I6690-02 - 1	BAYWAY-PHASE-3	0	-0.0149	-	7470A	PPB	05 Dec 2017 10:58:07	U	SMPL
I6699-04 - 1	RT-3874	12	-0.0114	-	7470A	PPB	05 Dec 2017 11:00:14	U	SMPL
I6701-02 - 1	MOBILE-TRANSFORMER-CONTAINMENT	11	-0.0117	-	7470A	PPB	05 Dec 2017 11:02:21	U	SMPL
PB104694BL - 1	PBW	21	-0.0088	-	7470A	PPB	05 Dec 2017 11:04:28	U	SMPL
PB104694BS - 1	LCSW	13361	3.8624	-	7470A	PPB	05 Dec 2017 11:06:36	U	SMPL
I6620-07 - 1	FB-1-20171128	-166	-0.0631	-	7470A	PPB	05 Dec 2017 11:08:44	U	SMPL
I6690-01 - 1	BAYWAY-PHASE-3	287	0.0684	-	7470A	PPB	05 Dec 2017 11:10:51	U	SMPL
I6690-01DUP - 1	BAYWAY-PHASE-3DUP	250	0.0577	-	7470A	PPB	05 Dec 2017 11:12:58	U	SMPL
I6690-01MS - 1	BAYWAY-PHASE-3MS	16215	4.6906	-	7470A	PPB	05 Dec 2017 11:15:06	U	SMPL
CCV46 - 1	CCV46	17215	4.9808	-	7470A	PPB	05 Dec 2017 11:17:14	U	SMPL
CCB46 - 1	CCB46	-90	-0.0410	-	7470A	PPB	05 Dec 2017 11:19:22	U	SMPL
I6690-01MSD - 1	BAYWAY-PHASE-3MSD	16549	4.7875	-	7470A	PPB	05 Dec 2017 11:21:30	U	SMPL
I6693-01 - 1	MW-14	-151	-0.0587	-	7470A	PPB	05 Dec 2017 11:23:37	U	SMPL
I6693-02 - 1	MW-6R	-48	-0.0288	-	7470A	PPB	05 Dec 2017 11:25:45	U	SMPL
I6693-03 - 1	MW-2	-15	-0.0192	-	7470A	PPB	05 Dec 2017 11:27:52	U	SMPL
I6693-04 - 1	MW-12	-14	-0.0189	-	7470A	PPB	05 Dec 2017 11:29:59	U	SMPL
I6701-01 - 1	MOBILE-TRANSFORMER-CONTAINMENT	-20	-0.0207	-	7470A	PPB	05 Dec 2017 11:32:07	U	SMPL
I6308-02LX5 - 1		18	-0.0097	-	7470A	PPB	05 Dec 2017 11:34:14	U	SMPL
I6308-02A - 1		14281	4.1294	-	7470A	PPB	05 Dec 2017 11:36:22	U	SMPL
I6690-01LX5 - 1		-25	-0.0221	-	7470A	PPB	05 Dec 2017 11:38:29	U	SMPL
I6690-01A - 1		16750	4.8459	-	7470A	PPB	05 Dec 2017 11:40:37	U	SMPL
CCV47 - 1	CCV47	17597	5.0917	-	7470A	PPB	05 Dec 2017 11:42:44	U	SMPL
CCB47 - 1	CCB47	-105	-0.0453	-	7470A	PPB	05 Dec 2017 11:44:52	U	SMPL
							05 Dec 2017 11:51:07	U	SMPL