


7470A

LB92096
INSTRUMENT ID: CV2

Linear

 μ Abs.:

36326

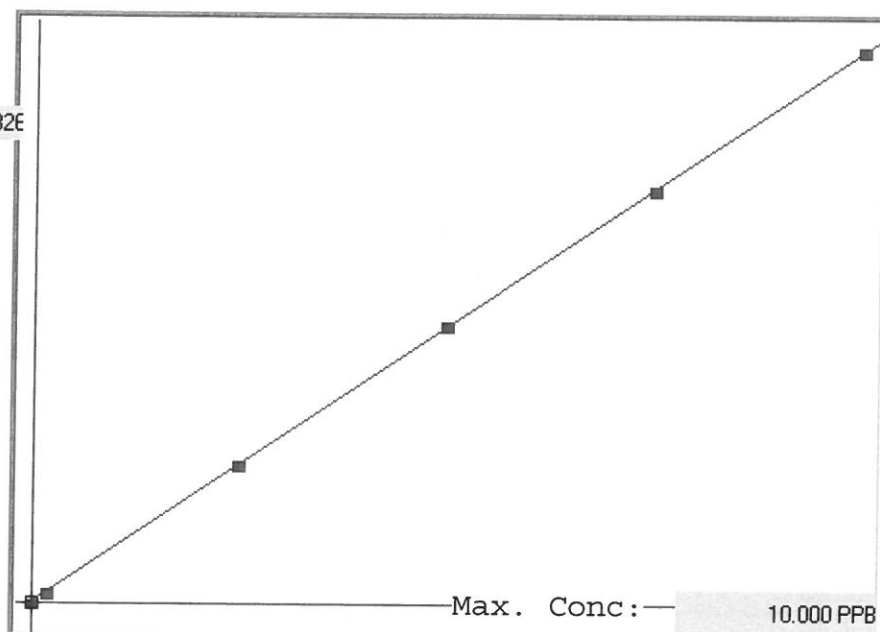

A= 0.0000e+000

B= 2.7576e-004

C= -1.3261e-002

Rho= 0.9999902

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.001	0.001	52	0.000	52				
0.2	0.200	0.183	-0.017	713	0.0 %	713				
2.5	2.500	2.514	0.014	9164	0.0 %	9164				
5.0	5.000	5.022	0.022	18261	0.0 %	18261				
7.5	7.500	7.475	-0.025	27156	0.0 %	27156				
10.0	10.000	10.004	0.004	36326	0.0 %	36326				

LB92096 INSTRUMENT ID : CV1

Method: 7470A		Operator: Admin		Date of Analysis: 12 Dec 2017 09:04:45				
Sample ID	Extended ID	µ Abs.	Conc.	Std ConcMethod	Units	Date	Type	Type
0.0 - 1	50	52	-	0.00007470A	PPB	12 Dec 2017 09:09:29	S	Std
0.2 - 1	50.2	713	-	0.20007470A	PPB	12 Dec 2017 09:11:39	S	Std
2.5 - 1	52.5	9164	-	2.50007470A	PPB	12 Dec 2017 09:13:47	S	Std
5.0 - 1	55	18261	-	5.00007470A	PPB	12 Dec 2017 09:15:55	S	Std
7.5 - 1	57.5	27156	-	7.50007470A	PPB	12 Dec 2017 09:18:03	S	Std
10.0 - 1	510	36326	-	10.00007470A	PPB	12 Dec 2017 09:20:11	S	Std
ICV04 - 1	ICV04	13886	3.8160	-7470A	PPB	12 Dec 2017 09:23:09	U	SMPL
ICB04 - 1	ICB04	-78	-0.0348	-7470A	PPB	12 Dec 2017 09:25:16	U	SMPL
CCV22 - 1	CCV22	18016	4.9548	-7470A	PPB	12 Dec 2017 09:27:22	U	SMPL
CCB22 - 1	CCB22	-100	-0.0408	-7470A	PPB	12 Dec 2017 09:29:29	U	SMPL
CRA - 1	CRA	704	0.1809	-7470A	PPB	12 Dec 2017 09:31:37	U	SMPL
HighStd - 1	HighStd	35585	9.7997	-7470A	PPB	12 Dec 2017 09:33:43	U	SMPL
ChkStd - 1	ChkStd	25357	6.9792	-7470A	PPB	12 Dec 2017 09:35:50	U	SMPL
PB104909BL - 1	PBW	-74	-0.0337	-7470A	PPB	12 Dec 2017 09:37:59	U	SMPL
PB104909BS - 1	LCSW	14471	3.9773	-7470A	PPB	12 Dec 2017 09:40:08	U	SMPL
PB104909TB - 1	PB104873TB	-59	-0.0295	-7470A	PPB	12 Dec 2017 09:42:16	U	SMPL
I6789-04 - 1	SP-1	94	0.0127	-7470A	PPB	12 Dec 2017 09:44:24	U	SMPL
I6789-04DUP - 1	SP-1DUP	149	0.0278	-7470A	PPB	12 Dec 2017 09:46:32	U	SMPL
I6789-04MS - 1	SP-1MS	13264	3.6444	-7470A	PPB	12 Dec 2017 09:48:41	U	SMPL
I6789-04MSD - 1	SP-1MSD	13466	3.7001	-7470A	PPB	12 Dec 2017 09:50:47	U	SMPL
CCV23 - 1	CCV23	18170	4.9973	-7470A	PPB	12 Dec 2017 09:52:55	U	SMPL
CCB23 - 1	CCB23	-97	-0.0400	-7470A	PPB	12 Dec 2017 09:55:01	U	SMPL
PB104910BL - 1	PBW	36	-0.0033	-7470A	PPB	12 Dec 2017 09:57:09	U	SMPL
PB104910BS - 1	LCSW	12984	3.5672	-7470A	PPB	12 Dec 2017 09:59:15	U	SMPL
PB104910TB - 1	PB104874TB	-26	-0.0204	-7470A	PPB	12 Dec 2017 10:01:22	U	SMPL
I6802-02 - 1	CONCRETE-17273	52	0.0011	-7470A	PPB	12 Dec 2017 10:03:29	U	SMPL
I6813-02 - 1	Soil-Cuttings	17	-0.0086	-7470A	PPB	12 Dec 2017 10:05:36	U	SMPL
I6813-04 - 1	Drill-Cutting-Spoils	54	0.0016	-7470A	PPB	12 Dec 2017 10:07:44	U	SMPL
I6814-04 - 1	PHMHC-WC1	145	0.0267	-7470A	PPB	12 Dec 2017 10:09:52	U	SMPL
I6814-04DUP - 1	PHMHC-WC1DUP	137	0.0245	-7470A	PPB	12 Dec 2017 10:12:00	U	SMPL
I6814-04MS - 1	PHMHC-WC1MS	13091	3.5967	-7470A	PPB	12 Dec 2017 10:14:09	U	SMPL
I6814-04MSD - 1	PHMHC-WC1MSD	13423	3.6883	-7470A	PPB	12 Dec 2017 10:16:16	U	SMPL
CCV24 - 1	CCV24	18373	5.0533	-7470A	PPB	12 Dec 2017 10:18:22	U	SMPL
CCB24 - 1	CCB24	-107	-0.0428	-7470A	PPB	12 Dec 2017 10:20:30	U	SMPL
PB104911BL - 1	PBW	34	-0.0039	-7470A	PPB	12 Dec 2017 10:22:38	U	SMPL
PB104911BS - 1	LCSW	13138	3.6097	-7470A	PPB	12 Dec 2017 10:24:45	U	SMPL
I6813-03 - 1	Drill-Cutting-Spoils	7	-0.0113	-7470A	PPB	12 Dec 2017 10:26:52	U	SMPL
I6824-01 - 1	TW-1	314	0.0733	-7470A	PPB	12 Dec 2017 10:28:59	U	SMPL
I6824-03 - 1	TW-4	986	0.2586	-7470A	PPB	12 Dec 2017 10:31:06	U	SMPL
I6824-04 - 1	TW-3	10611	2.9128	-7470A	PPB	12 Dec 2017 10:33:14	U	SMPL
I6824-05 - 1	TW-2	22524	6.1980	-7470A	PPB	12 Dec 2017 10:35:22	U	SMPL
I6833-01 - 1	MW-2A	-92	-0.0386	-7470A	PPB	12 Dec 2017 10:37:30	U	SMPL
I6833-02 - 1	DUP1	6	-0.0116	-7470A	PPB	12 Dec 2017 10:39:39	U	SMPL
I6833-04 - 1	MW-6	1054	0.2774	-7470A	PPB	12 Dec 2017 10:41:47	U	SMPL
CCV25 - 1	CCV25	17963	4.9402	-7470A	PPB	12 Dec 2017 10:43:54	U	SMPL
CCB25 - 1	CCB25	-57	-0.0290	-7470A	PPB	12 Dec 2017 10:46:01	U	SMPL
I6833-04DUP - 1	MW-6DUP	1044	0.2746	-7470A	PPB	12 Dec 2017 10:48:09	U	SMPL
I6833-05 - 1	I6833-04MS	16636	4.5743	-7470A	PPB	12 Dec 2017 10:50:16	U	SMPL
I6833-06 - 1	I6833-04MSD	16160	4.4430	-7470A	PPB	12 Dec 2017 10:52:23	U	SMPL
I6833-07 - 1	MW-13	1214	0.3215	-7470A	PPB	12 Dec 2017 10:54:31	U	SMPL
I6833-08 - 1	MW-9	1053	0.2771	-7470A	PPB	12 Dec 2017 10:56:39	U	SMPL
I6833-09 - 1	MW-7	78	0.0082	-7470A	PPB	12 Dec 2017 10:58:47	U	SMPL
I6833-10 - 1	MW-16	198	0.0413	-7470A	PPB	12 Dec 2017 11:00:55	U	SMPL
CCV26 - 1	CCV26	18159	4.9943	-7470A	PPB	12 Dec 2017 11:03:03	U	SMPL
CCB26 - 1	CCB26	-79	-0.0350	-7470A	PPB	12 Dec 2017 11:05:12	U	SMPL
I6789-04LX5 - 1		62	0.0038	-7470A	PPB	12 Dec 2017 11:07:19	U	SMPL
I6789-04A - 1		13445	3.6943	-7470A	PPB	12 Dec 2017 11:09:27	U	SMPL
I6814-04LX5 - 1		-33	-0.0224	-7470A	PPB	12 Dec 2017 11:11:34	U	SMPL
I6814-04A - 1		14029	3.8554	-7470A	PPB	12 Dec 2017 11:13:41	U	SMPL
I6833-04LX5 - 1		115	0.0185	-7470A	PPB	12 Dec 2017 11:15:49	U	SMPL
I6833-04A - 1		15791	4.3413	-7470A	PPB	12 Dec 2017 11:17:56	U	SMPL
CCV27 - 1	CCV27	17958	4.9389	-7470A	PPB	12 Dec 2017 11:20:03	U	SMPL
CCB27 - 1	CCB27	-47	-0.0262	-7470A	PPB	12 Dec 2017 11:22:11	U	SMPL