


7470A

LB 92158
INSTRUMENT ID: CY1

Linear

 μ Abs.:

35537

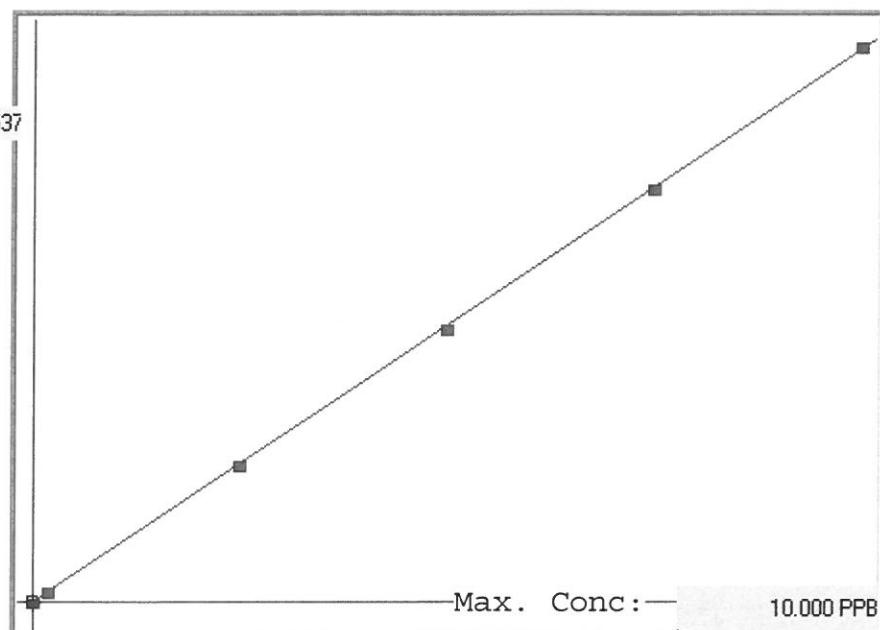

A= 0.0000e+000

B= 2.8218e-004

C= 9.2439e-003

Rho= 0.9999690

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.023	0.023	48	0.000	48				
0.2	0.200	0.213	0.013	721	0.0 %	721				
2.5	2.500	2.493	-0.007	8803	0.0 %	8803				
5.0	5.000	4.947	-0.053	17499	0.0 %	17499				
7.5	7.500	7.487	-0.013	26499	0.0 %	26499				
10.0	10.000	10.037	0.037	35537	0.0 %	35537				

LB92158 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 14 Dec 2017 10:28:57

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	48	-	0.0000	7470A	PPB	14 Dec 2017 10:29:23	S	Std
0.2 - 1	50.2	721	-	0.2000	7470A	PPB	14 Dec 2017 10:31:31	S	Std
2.5 - 1	52.5	8803	-	2.5000	7470A	PPB	14 Dec 2017 10:33:40	S	Std
5.0 - 1	55	17499	-	5.0000	7470A	PPB	14 Dec 2017 10:35:48	S	Std
7.5 - 1	57.5	26499	-	7.5000	7470A	PPB	14 Dec 2017 10:37:56	S	Std
10.0 - 1	57.5	35537	-	10.0000	7470A	PPB	14 Dec 2017 10:40:04	S	Std
ICV09 - 1	ICV09	13685	3.8709	-	7470A	PPB	14 Dec 2017 10:42:34	U	SMPL
ICB09 - 1	ICB09	-77	-0.0125	-	7470A	PPB	14 Dec 2017 10:44:40	U	SMPL
CCV58 - 1	CCV58	17534	4.9571	-	7470A	PPB	14 Dec 2017 10:46:48	U	SMPL
CCB58 - 1	CCB58	-79	-0.0130	-	7470A	PPB	14 Dec 2017 10:48:54	U	SMPL
CRA - 1	CRA	739	0.2178	-	7470A	PPB	14 Dec 2017 10:51:02	U	SMPL
HighStd - 1	HighStd	35229	9.9503	-	7470A	PPB	14 Dec 2017 10:53:08	U	SMPL
ChkStd - 1	ChkStd	24524	6.9295	-	7470A	PPB	14 Dec 2017 10:55:15	U	SMPL
PB105009BL - 1	PBW	-87	-0.0153	-	7470A	PPB	14 Dec 2017 10:57:24	U	SMPL
PB105009BS - 1	LCSW	13367	3.7812	-	7470A	PPB	14 Dec 2017 11:03:23	U	SMPL
PB105009TB - 1	PB104975TB	-75	-0.0119	-	7470A	PPB	14 Dec 2017 11:05:30	U	SMPL
I6886-04 - 1	TR-04-121117	16	0.0138	-	7470A	PPB	14 Dec 2017 11:07:39	U	SMPL
I6886-04DUP - 1	TR-04-121117DUP	19	0.0146	-	7470A	PPB	14 Dec 2017 11:09:47	U	SMPL
I6886-04MS - 1	TR-04-121117MS	13326	3.7696	-	7470A	PPB	14 Dec 2017 11:14:18	U	SMPL
I6886-04MSD - 1	TR-04-121117MSD	13121	3.7118	-	7470A	PPB	14 Dec 2017 11:16:24	U	SMPL
CCV59 - 1	CCV59	17880	5.0547	-	7470A	PPB	14 Dec 2017 11:18:30	U	SMPL
CCB59 - 1	CCB59	-74	-0.0116	-	7470A	PPB	14 Dec 2017 11:20:38	U	SMPL
I6885-03 - 1	WC-003	22	0.0155	-	7470A	PPB	14 Dec 2017 11:22:45	U	SMPL
PB105010BL - 1	PBW	23	0.0157	-	7470A	PPB	14 Dec 2017 11:24:52	U	SMPL
PB105010BS - 1	LCSW	13233	3.7434	-	7470A	PPB	14 Dec 2017 11:30:47	U	SMPL
I6878-01 - 1	TW-5	163	0.0552	-	7470A	PPB	14 Dec 2017 11:32:54	U	SMPL
I6878-04 - 1	TW-5	7	0.0112	-	7470A	PPB	14 Dec 2017 11:35:01	U	SMPL
I6883-02 - 1	FB-02	9	0.0118	-	7470A	PPB	14 Dec 2017 11:37:09	U	SMPL
I6884-02 - 1	MW-1-20171211	284	0.0894	-	7470A	PPB	14 Dec 2017 11:39:17	U	SMPL
I6884-02DUP - 1	MW-1-20171211DUP	311	0.0970	-	7470A	PPB	14 Dec 2017 11:41:25	U	SMPL
I6884-03 - 1	I6884-02MS	13894	3.9299	-	7470A	PPB	14 Dec 2017 11:43:34	U	SMPL
I6884-04 - 1	I6884-02MSD	13741	3.8867	-	7470A	PPB	14 Dec 2017 11:45:41	U	SMPL
CCV60 - 1	CCV60	17588	4.9723	-	7470A	PPB	14 Dec 2017 11:47:47	U	SMPL
CCB60 - 1	CCB60	-80	-0.0133	-	7470A	PPB	14 Dec 2017 11:49:54	U	SMPL
I6884-05 - 1	MW-4-20171211	305	0.0953	-	7470A	PPB	14 Dec 2017 11:52:02	U	SMPL
I6884-06 - 1	MW-X-20171211	339	0.1049	-	7470A	PPB	14 Dec 2017 11:54:09	U	SMPL
I6884-07 - 1	FB-20171211	61	0.0265	-	7470A	PPB	14 Dec 2017 11:56:16	U	SMPL
I6884-08 - 1	MW-11-20171211	306	0.0956	-	7470A	PPB	14 Dec 2017 11:58:23	U	SMPL
I6884-09 - 1	MW-1-20171211	310	0.0967	-	7470A	PPB	14 Dec 2017 12:00:30	U	SMPL
I6884-10 - 1	I6884-09MS	14436	4.0828	-	7470A	PPB	14 Dec 2017 12:02:38	U	SMPL
I6884-11 - 1	I6884-09MSD	14889	4.2107	-	7470A	PPB	14 Dec 2017 12:04:46	U	SMPL
I6884-12 - 1	MW-4-20171211	128	0.0454	-	7470A	PPB	14 Dec 2017 12:06:54	U	SMPL
I6884-13 - 1	MW-X-20171211	301	0.0942	-	7470A	PPB	14 Dec 2017 12:09:03	U	SMPL
I6884-15 - 1	MW-11-20171211	323	0.1004	-	7470A	PPB	14 Dec 2017 12:11:10	U	SMPL
CCV61 - 1	CCV61	17893	5.0584	-	7470A	PPB	14 Dec 2017 12:13:17	U	SMPL
CCB61 - 1	CCB61	-70	-0.0105	-	7470A	PPB	14 Dec 2017 12:15:25	U	SMPL
I6886-04LX5 - 1		37	0.0197	-	7470A	PPB	14 Dec 2017 12:17:33	U	SMPL
I6886-04A - 1		14149	4.0019	-	7470A	PPB	14 Dec 2017 12:19:40	U	SMPL
I6884-02LX5 - 1		16	0.0138	-	7470A	PPB	14 Dec 2017 12:21:47	U	SMPL
I6884-02A - 1		14251	4.0306	-	7470A	PPB	14 Dec 2017 12:23:54	U	SMPL
CCV62 - 1	CCV62	17665	4.9940	-	7470A	PPB	14 Dec 2017 12:26:02	U	SMPL
CCB62 - 1	CCB62	-64	-0.0088	-	7470A	PPB	14 Dec 2017 12:28:09	U	SMPL