


7471A

LB 92303
INSTRUMENT ID: CV2

Linear

 μ Abs.:

42515

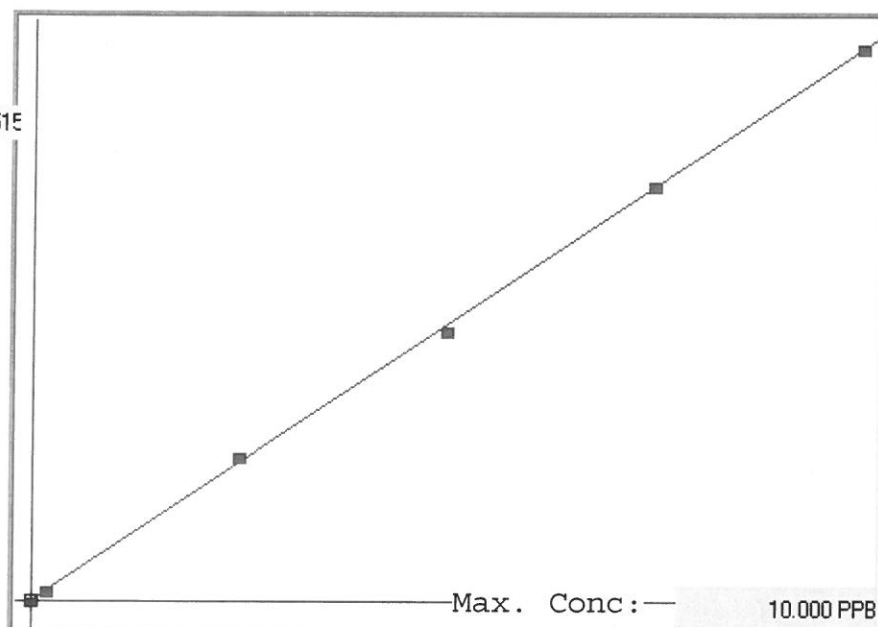

A= 0.0000e+000

B= 2.3548e-004

C= -5.2855e-003

Rho= 0.9998474

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.002	-0.002	13	0.000	13				
0.2	0.200	0.183	-0.017	798	0.0 %	798				
2.5	2.500	2.596	0.096	11047	0.0 %	11047				
5.0	5.000	4.881	-0.119	20752	0.0 %	20752				
7.5	7.500	7.536	0.036	32025	0.0 %	32025	0			
10.0	10.000	10.006	0.006	42515	0.0 %	42515				

LB92303 INSTRUMENT ID : CV1

Method: 7471A

Operator: Admin

Date of Analysis: 21 Dec 2017 09:15:14

Sample ID	Extended ID	μ Abs	Conc	Std CondMethod	Units	Date	Type	Type
0.0 - 1	SO	13	-	0.00007471A	PPB	21 Dec 2017 09:32:49	S	Std
0.2 - 1	SO.2	798	-	0.20007471A	PPB	21 Dec 2017 09:35:07	S	Std
2.5 - 1	SO.5	11047	-	2.50007471A	PPB	21 Dec 2017 09:37:24	S	Std
5.0 - 1	SO.5	20752	-	5.00007471A	PPB	21 Dec 2017 09:39:42	S	Std
7.5 - 1	SO.5	32025	-	7.50007471A	PPB	21 Dec 2017 09:41:59	S	Std
10.0 - 1	SO	42515	-	10.00007471A	PPB	21 Dec 2017 09:44:17	S	Std
ICV18 - 1	ICV18	16802	3.9513	-7471A	PPB	21 Dec 2017 09:47:02	U	SMPL
ICB18 - 1	ICB18	-146	-0.0397	-7471A	PPB	21 Dec 2017 09:49:18	U	SMPL
CCV19 - 1	CCV19	20385	4.7950	-7471A	PPB	21 Dec 2017 09:51:33	U	SMPL
CCB19 - 1	CCB19	-100	-0.0288	-7471A	PPB	21 Dec 2017 09:53:49	U	SMPL
CRA - 1	CRA	802	0.1836	-7471A	PPB	21 Dec 2017 09:56:06	U	SMPL
HighStd - 1	HighStd	42882	10.0926	-7471A	PPB	21 Dec 2017 09:58:22	U	SMPL
ChkStd - 1	ChkStd	29629	6.9718	-7471A	PPB	21 Dec 2017 10:00:37	U	SMPL
PB105189BL - 1	PBS	-102	-0.0293	-7471A	PPB	21 Dec 2017 10:02:56	U	SMPL
PB105189BS - 1	LCSS	14855	3.4928	-7471A	PPB	21 Dec 2017 10:05:14	U	SMPL
I6676-08 - 1	OK-01-121817	462	0.1035	-7471A	PPB	21 Dec 2017 10:07:31	U	SMPL
I6682-01 - 1	NB-01-121817-A	1020	0.2349	-7471A	PPB	21 Dec 2017 10:09:48	U	SMPL
I6682-03 - 1	NB-01-121817-B	1023	0.2356	-7471A	PPB	21 Dec 2017 10:12:05	U	SMPL
I6682-05 - 1	NB-01-121817-C	2006	0.4671	-7471A	PPB	21 Dec 2017 10:14:23	U	SMPL
I6981-01 - 1	PHMHA-WCS	15221	3.5790	-7471A	PPB	21 Dec 2017 10:16:39	U	SMPL
CCV20 - 1	CCV20	20153	4.7403	-7471A	PPB	21 Dec 2017 10:18:55	U	SMPL
CCB20 - 1	CCB20	-119	-0.0333	-7471A	PPB	21 Dec 2017 10:21:10	U	SMPL
I6981-04 - 1	PHMHA-WCD	12516	2.9420	-7471A	PPB	21 Dec 2017 10:23:26	U	SMPL
I6981-07 - 1	PHMHB-WCS	14610	3.4351	-7471A	PPB	21 Dec 2017 10:25:42	U	SMPL
I6981-10 - 1	PHMHB-WCD	6172	1.4481	-7471A	PPB	21 Dec 2017 10:27:58	U	SMPL
I6988-01 - 1	RT4008-RT3867-RT3075	1753	0.4075	-7471A	PPB	21 Dec 2017 10:30:14	U	SMPL
I6988-01DUP - 1	RT4008-RT3867-RT3075DUP	1869	0.4348	-7471A	PPB	21 Dec 2017 10:32:31	U	SMPL
I6988-01MS - 1	RT4008-RT3867-RT3075MS	16684	3.9235	-7471A	PPB	21 Dec 2017 10:34:48	U	SMPL
I6988-01MSD - 1	RT4008-RT3867-RT3075MSD	17293	4.0669	-7471A	PPB	21 Dec 2017 10:37:05	U	SMPL
I6990-01 - 1	MH-CONCRETE	1132	0.2613	-7471A	PPB	21 Dec 2017 10:39:23	U	SMPL
I6993-01 - 1	ROLL-OFF-3	1142	0.2636	-7471A	PPB	21 Dec 2017 10:41:40	U	SMPL
I6993-02 - 1	ROLL-OFF-4	6524	1.5310	-7471A	PPB	21 Dec 2017 10:43:56	U	SMPL
CCV21 - 1	CCV21	20165	4.7432	-7471A	PPB	21 Dec 2017 10:46:12	U	SMPL
CCB21 - 1	CCB21	-121	-0.0338	-7471A	PPB	21 Dec 2017 10:48:29	U	SMPL
I6995-01 - 1	TP-1	2476	0.5778	-7471A	PPB	21 Dec 2017 10:50:46	U	SMPL
I6995-02 - 1	TP-2	11884	2.7932	-7471A	PPB	21 Dec 2017 10:53:02	U	SMPL
PB105235BL - 1	PBS	-52	-0.0175	-7471A	PPB	21 Dec 2017 10:55:18	U	SMPL
PB105235BS - 1	LCSS	14788	3.4770	-7471A	PPB	21 Dec 2017 10:57:35	U	SMPL
I6997-01 - 1	EP-02	3110	0.7271	-7471A	PPB	21 Dec 2017 11:05:02	U	SMPL
I6997-01DUP - 1	EP-02DUP	3014	0.7045	-7471A	PPB	21 Dec 2017 11:07:18	U	SMPL
I6997-02 - 1	I6997-01MS	20079	4.7229	-7471A	PPB	21 Dec 2017 11:09:35	U	SMPL
I6997-03 - 1	I6997-01MSD	19124	4.4980	-7471A	PPB	21 Dec 2017 11:11:53	U	SMPL
I6997-04 - 1	EP-10	224	0.0475	-7471A	PPB	21 Dec 2017 11:14:11	U	SMPL
I6997-05 - 1	EP-18	456	0.1021	-7471A	PPB	21 Dec 2017 11:16:28	U	SMPL
CCV22 - 1	CCV22	20264	4.7665	-7471A	PPB	21 Dec 2017 11:18:44	U	SMPL
CCB22 - 1	CCB22	-106	-0.0302	-7471A	PPB	21 Dec 2017 11:21:01	U	SMPL
I6997-06 - 1	EP-26	1161	0.2681	-7471A	PPB	21 Dec 2017 11:23:18	U	SMPL
I6997-07 - 1	EP-29	370	0.0818	-7471A	PPB	21 Dec 2017 11:25:35	U	SMPL
I6997-08 - 1	EP-32	2561	0.5978	-7471A	PPB	21 Dec 2017 11:27:51	U	SMPL
I6997-09 - 1	BLIND-DUPLICATE	387	0.0858	-7471A	PPB	21 Dec 2017 11:30:08	U	SMPL
I7002-01 - 1	EPE-106-3DS(16-20)	10469	2.4600	-7471A	PPB	21 Dec 2017 11:32:24	U	SMPL
I7002-02 - 1	EPE-106-3DS(20-30)	-7	-0.0069	-7471A	PPB	21 Dec 2017 11:34:41	U	SMPL
I7002-03 - 1	EPE-106-3DS(32-40)	107	0.0199	-7471A	PPB	21 Dec 2017 11:36:59	U	SMPL
I7002-04 - 1	EPE-106-3DS(40-50)	47	0.0058	-7471A	PPB	21 Dec 2017 11:39:16	U	SMPL
I7002-05 - 1	EPE-106-3DS(55-67)	301	0.0656	-7471A	PPB	21 Dec 2017 11:41:34	U	SMPL
I7002-06 - 1	EPE-106-3DS(67-77)	90	0.0159	-7471A	PPB	21 Dec 2017 11:43:50	U	SMPL
CCV23 - 1	CCV23	21096	4.9624	-7471A	PPB	21 Dec 2017 11:46:07	U	SMPL
CCB23 - 1	CCB23	-132	-0.0364	-7471A	PPB	21 Dec 2017 11:48:23	U	SMPL
I7002-07 - 1	EPE-106-3DS(60-62)	411	0.0915	-7471A	PPB	21 Dec 2017 11:50:40	U	SMPL
I7002-08 - 1	EPE-106-3DS(65-67)	450	0.1007	-7471A	PPB	21 Dec 2017 11:52:57	U	SMPL
I7002-09 - 1	EPE-106-3DS(72-74)	724	0.1652	-7471A	PPB	21 Dec 2017 11:55:13	U	SMPL
I7002-10 - 1	EPE-106-3DS(75-77)	502	0.1129	-7471A	PPB	21 Dec 2017 11:57:29	U	SMPL
I7002-11 - 1	EPE-106-3DS(85-87)	620	0.1407	-7471A	PPB	21 Dec 2017 11:59:46	U	SMPL
I7006-01 - 1	TB-07(6-8)	168060	39.5695	-7471A	PPB	21 Dec 2017 12:02:03	U	SMPL
I7019-01 - 1	EP-27	-241	-0.0620	-7471A	PPB	21 Dec 2017 12:04:20	U	SMPL
PB105236BL - 1	PBS	-14	-0.0086	-7471A	PPB	21 Dec 2017 12:06:47	U	SMPL
PB105236BS - 1	LCSS	14784	3.4761	-7471A	PPB	21 Dec 2017 12:09:05	U	SMPL
I6681-01 - 1	PL-01-121917-A	852	0.1953	-7471A	PPB	21 Dec 2017 12:11:21	U	SMPL
CCV24 - 1	CCV24	20955	4.9292	-7471A	PPB	21 Dec 2017 12:13:38	U	SMPL
CCB24 - 1	CCB24	-128	-0.0354	-7471A	PPB	21 Dec 2017 12:15:54	U	SMPL
I6681-01DUP - 1	PL-01-121917-ADUP	808	0.1850	-7471A	PPB	21 Dec 2017 12:20:49	U	SMPL
I6681-01MS - 1	PL-01-121917-AMS	15330	3.6046	-7471A	PPB	21 Dec 2017 12:23:05	U	SMPL
I6681-01MSD - 1	PL-01-121917-AMSD	15835	3.7235	-7471A	PPB	21 Dec 2017 12:25:21	U	SMPL
I6681-03 - 1	PL-01-121917-B	252	0.0541	-7471A	PPB	21 Dec 2017 12:27:38	U	SMPL
I6681-05 - 1	PL-01-121917-C	937	0.2154	-7471A	PPB	21 Dec 2017 12:29:55	U	SMPL
I6681-07 - 1	PL-01-121917-D	994	0.2288	-7471A	PPB	21 Dec 2017 12:32:12	U	SMPL
I6683-07 - 1	EO-02-122017-A	6458	1.5154	-7471A	PPB	21 Dec 2017 12:34:29	U	SMPL
I6683-09 - 1	EO-02-122017-B	666	0.1515	-7471A	PPB	21 Dec 2017 12:36:47	U	SMPL
I6683-11 - 1	EO-02-122017-C	2013	0.4687	-7471A	PPB	21 Dec 2017 12:39:04	U	SMPL
CCV25 - 1	CCV25	21071	4.9565	-7471A	PPB	21 Dec 2017 12:41:21	U	SMPL
CCB25 - 1	CCB25	-107	-0.0305	-7471A	PPB	21 Dec 2017 12:43:38	U	SMPL
I9988-01LX5 - 1		317	0.0694	-7471A	PPB	21 Dec 2017 12:45:56	U	SMPL
I9988-01A - 1		17803	4.1870	-7471A	PPB	21 Dec 2017 12:48:13	U	SMPL
I9997-01LX5 - 1		462	0.1035	-7471A	PPB	21 Dec 2017 12:50:30	U	SMPL
I9997-01A - 1		18783	4.4177	-7471A	PPB	21 Dec 2017 12:52:47	U	SMPL
I6681-01LX5 - 1		69	0.0110	-7471A	PPB	21 Dec 2017 12:55:05	U	SMPL
I6681-01A - 1		16322	3.8382	-7471A	PPB	21 Dec 2017 12:57:22	U	SMPL
I7006-01DLX10 - 1		17039	4.0071	-7471A	PPB	21 Dec 2017 12:59:39	U	SMPL
CCV26 - 1	CCV26	20777	4.8873	-7471A	PPB	21 Dec 2017 13:01:56	U	SMPL
CCB26 - 1	CCB26	-137	-0.0375	-7471A	PPB	21 Dec 2017 13:04:13	U	SMPL