


7470A

LB 92936
INSTRUMENT ID: CV1

Linear

 μ Abs.:

35817

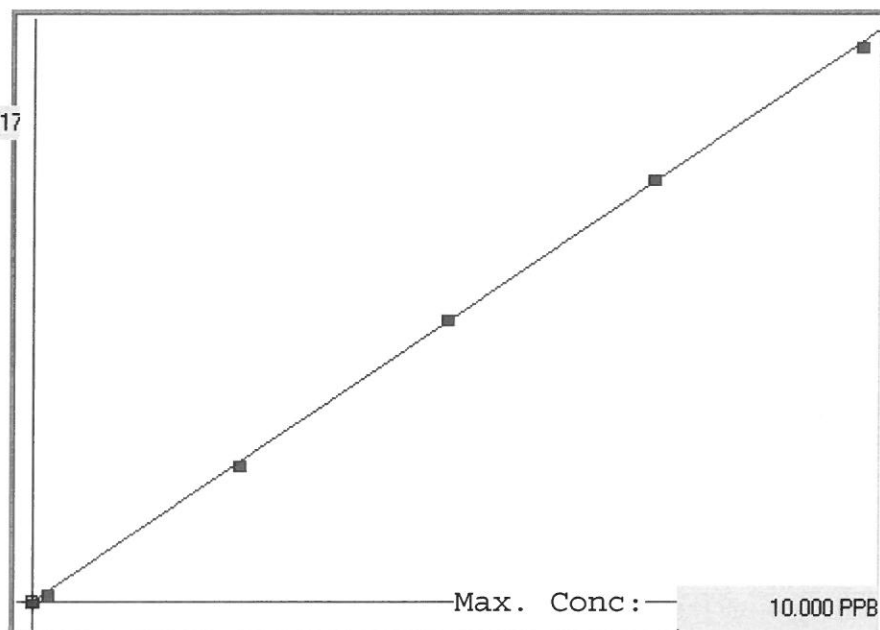

A= 0.0000e+000

B= 2.7669e-004

C= 1.0340e-002

Rho= 0.9998876

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.010	0.010	0	0.000	0				
0.2	0.200	0.172	-0.028	584	0.0 %	584				
2.5	2.500	2.461	-0.039	8856	0.0 %	8856				
5.0	5.000	5.057	0.057	18241	0.0 %	18241				
7.5	7.500	7.579	0.079	27356	0.0 %	27356				
10.0	10.000	9.920	-0.080	35817	0.0 %	35817				

LB92936 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 27 Jan 2018 12:19:15

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	0	-	0.0000	7470A	PPB	27 Jan 2018 12:23:32	S	Std
0.2 - 1	50.2	584	-	0.2000	7470A	PPB	27 Jan 2018 12:25:40	S	Std
2.5 - 1	52.5	8856	-	2.5000	7470A	PPB	27 Jan 2018 12:27:49	S	Std
5.0 - 1	55	18241	-	5.0000	7470A	PPB	27 Jan 2018 12:29:57	S	Std
7.5 - 1	57.5	27356	-	7.5000	7470A	PPB	27 Jan 2018 12:32:05	S	Std
10.0 - 1	50	35817	-	10.0000	7470A	PPB	27 Jan 2018 12:36:39	S	Std
ICV68 - 1	ICV68	14089	3.9086	-	7470A	PPB	27 Jan 2018 12:39:16	U	SMPL
ICB68 - 1	ICB68	-107	-0.0193	-	7470A	PPB	27 Jan 2018 12:41:23	U	SMPL
CCV01 - 1	CCV01	17920	4.9685	-	7470A	PPB	27 Jan 2018 12:43:30	U	SMPL
CCB01 - 1	CCB01	-62	-0.0068	-	7470A	PPB	27 Jan 2018 12:45:36	U	SMPL
CRA - 1	CRA	591	0.1739	-	7470A	PPB	27 Jan 2018 12:47:43	U	SMPL
HighStd - 1	HighStd	36253	10.0410	-	7470A	PPB	27 Jan 2018 12:49:50	U	SMPL
ChkStd - 1	ChkStd	24760	6.8611	-	7470A	PPB	27 Jan 2018 12:51:56	U	SMPL
PB106106BL - 1	PBW	-73	-0.0099	-	7470A	PPB	27 Jan 2018 12:56:30	U	SMPL
PB106106BS - 1	LCSW	12917	3.5843	-	7470A	PPB	27 Jan 2018 12:58:38	U	SMPL
PB106106TB - 1	PB106023TB	-146	-0.0301	-	7470A	PPB	27 Jan 2018 13:00:45	U	SMPL
J1010-09 - 1	BU-01-012518	-80	-0.0118	-	7470A	PPB	27 Jan 2018 13:02:53	U	SMPL
J1010-09DUP - 1	BU-01-012518DUP	-69	-0.0088	-	7470A	PPB	27 Jan 2018 13:05:02	U	SMPL
J1010-09MS - 1	BU-01-012518MS	13351	3.7044	-	7470A	PPB	27 Jan 2018 13:07:10	U	SMPL
J1010-09MSD - 1	BU-01-012518MSD	12882	3.5746	-	7470A	PPB	27 Jan 2018 13:09:16	U	SMPL
CCV02 - 1	CCV02	18332	5.0825	-	7470A	PPB	27 Jan 2018 13:11:22	U	SMPL
CCB02 - 1	CCB02	-129	-0.0254	-	7470A	PPB	27 Jan 2018 13:13:29	U	SMPL
J1018-11 - 1	OR-03-012518	-127	-0.0248	-	7470A	PPB	27 Jan 2018 13:15:37	U	SMPL
J1023-06 - 1	TR-05-012518	-87	-0.0137	-	7470A	PPB	27 Jan 2018 13:17:43	U	SMPL
J1307-04 - 1	MANHOLE-201	-68	-0.0085	-	7470A	PPB	27 Jan 2018 13:19:50	U	SMPL
J1310-01 - 1	CHVB0796	-89	-0.0143	-	7470A	PPB	27 Jan 2018 13:21:57	U	SMPL
J1311-01 - 1	19505-7	-48	-0.0029	-	7470A	PPB	27 Jan 2018 13:24:05	U	SMPL
J1311-02 - 1	19501-4	-18	0.0054	-	7470A	PPB	27 Jan 2018 13:26:12	U	SMPL
J1311-07 - 1	23318	-24	0.0037	-	7470A	PPB	27 Jan 2018 13:28:20	U	SMPL
J1311-08 - 1	19520-25-26-27-31	-37	0.0001	-	7470A	PPB	27 Jan 2018 13:30:28	U	SMPL
J1311-09 - 1	19521-22-23-24-30-44	36	0.0203	-	7470A	PPB	27 Jan 2018 13:32:37	U	SMPL
J1322-02 - 1	M3-LEFT-RIGHT	-91	-0.0148	-	7470A	PPB	27 Jan 2018 13:34:44	U	SMPL
CCV03 - 1	CCV03	18133	5.0275	-	7470A	PPB	27 Jan 2018 13:36:50	U	SMPL
CCB03 - 1	CCB03	-119	-0.0226	-	7470A	PPB	27 Jan 2018 13:38:56	U	SMPL
J1325-03 - 1	RO-4632	-105	-0.0187	-	7470A	PPB	27 Jan 2018 13:41:04	U	SMPL
J1325-06 - 1	RO-3025	-86	-0.0135	-	7470A	PPB	27 Jan 2018 13:43:11	U	SMPL
J1325-09 - 1	RO-2334	-14	0.0065	-	7470A	PPB	27 Jan 2018 13:45:18	U	SMPL
J1325-12 - 1	RO-2342	-66	-0.0079	-	7470A	PPB	27 Jan 2018 13:47:25	U	SMPL
J1326-02 - 1	RO200030	-79	-0.0115	-	7470A	PPB	27 Jan 2018 13:49:32	U	SMPL
J1328-03 - 1	RO-1-2	-82	-0.0123	-	7470A	PPB	27 Jan 2018 13:51:39	U	SMPL
PB106107BL - 1	PBW	-85	-0.0132	-	7470A	PPB	27 Jan 2018 13:53:47	U	SMPL
PB106107BS - 1	LCSW	13412	3.7212	-	7470A	PPB	27 Jan 2018 13:55:55	U	SMPL
PB106107TB - 1	PB106033TB	-146	-0.0301	-	7470A	PPB	27 Jan 2018 13:58:04	U	SMPL
J1009-02 - 1	AU-05-012518-A	-80	-0.0118	-	7470A	PPB	27 Jan 2018 14:00:10	U	SMPL
CCV04 - 1	CCV04	17933	4.9721	-	7470A	PPB	27 Jan 2018 14:02:18	U	SMPL
CCB04 - 1	CCB04	-153	-0.0320	-	7470A	PPB	27 Jan 2018 14:04:25	U	SMPL
J1009-02DUP - 1	AU-05-012518-ADUP	-95	-0.0159	-	7470A	PPB	27 Jan 2018 14:06:33	U	SMPL
J1009-02MS - 1	AU-05-012518-AMS	13640	3.7843	-	7470A	PPB	27 Jan 2018 14:08:39	U	SMPL
J1009-02MSD - 1	AU-05-012518-AMSD	13382	3.7129	-	7470A	PPB	27 Jan 2018 14:10:46	U	SMPL
J1009-04 - 1	AU-05-012518-B	-163	-0.0348	-	7470A	PPB	27 Jan 2018 14:12:54	U	SMPL
J1009-06 - 1	AU-05-012518-C	-130	-0.0256	-	7470A	PPB	27 Jan 2018 14:15:01	U	SMPL
J1009-08 - 1	AU-05-012518-D	-87	-0.0137	-	7470A	PPB	27 Jan 2018 14:17:09	U	SMPL
J1009-10 - 1	AU-06-012518-A	-95	-0.0159	-	7470A	PPB	27 Jan 2018 14:19:17	U	SMPL
J1009-12 - 1	AU-06-012518-B	-17	0.0056	-	7470A	PPB	27 Jan 2018 14:21:25	U	SMPL
J1009-14 - 1	AU-06-012518-C	-18	0.0054	-	7470A	PPB	27 Jan 2018 14:23:34	U	SMPL
J1303-01 - 1	CHASSIS-WASH	-52	-0.0040	-	7470A	PPB	27 Jan 2018 14:25:40	U	SMPL
CCV05 - 1	CCV05	17609	4.8825	-	7470A	PPB	27 Jan 2018 14:27:48	U	SMPL
CCB05 - 1	CCB05	-125	-0.0242	-	7470A	PPB	27 Jan 2018 14:29:55	U	SMPL
J1303-02 - 1	BUS-WASH-ZIPPER-DRAINS	-46	-0.0024	-	7470A	PPB	27 Jan 2018 14:32:03	U	SMPL
J1303-03 - 1	SLUDGE-PIT	3	0.0112	-	7470A	PPB	27 Jan 2018 14:34:10	U	SMPL
J1305-01 - 1	INTERIOR-ZIPPER-DRAIN	-31	0.0018	-	7470A	PPB	27 Jan 2018 14:36:17	U	SMPL
J1305-02 - 1	ENGINE-WASH	-70	-0.0090	-	7470A	PPB	27 Jan 2018 14:38:24	U	SMPL
J1305-03 - 1	OWS	-15	0.0062	-	7470A	PPB	27 Jan 2018 14:40:31	U	SMPL
J1305-04 - 1	BUS-WASH	-26	0.0031	-	7470A	PPB	27 Jan 2018 14:42:39	U	SMPL
J1305-05 - 1	RECLAIMER-SLUDGE-PIT	-11	0.0073	-	7470A	PPB	27 Jan 2018 14:44:46	U	SMPL
J1320-03 - 1	T1WC-1	-54	-0.0046	-	7470A	PPB	27 Jan 2018 14:46:55	U	SMPL
PB106109BL - 1	PBW	-43	-0.0016	-	7470A	PPB	27 Jan 2018 14:49:03	U	SMPL
PB106109BS - 1	LCSW	13309	3.6927	-	7470A	PPB	27 Jan 2018 14:51:10	U	SMPL
CCV06 - 1	CCV06	17792	4.9331	-	7470A	PPB	27 Jan 2018 14:53:18	U	SMPL
CCB06 - 1	CCB06	-150	-0.0312	-	7470A	PPB	27 Jan 2018 14:55:25	U	SMPL
PB106109TB - 1	PB106020TB	-209	-0.0475	-	7470A	PPB	27 Jan 2018 14:57:33	U	SMPL
J1261-01 - 1	WC-01(0-5)	374	0.1138	-	7470A	PPB	27 Jan 2018 14:59:41	U	SMPL
J1261-02 - 1	WC-02(0-5)	21	0.0162	-	7470A	PPB	27 Jan 2018 15:01:48	U	SMPL
J1261-03 - 1	WC-03(0-5)	-210	-0.0478	-	7470A	PPB	27 Jan 2018 15:03:55	U	SMPL
J1261-03DUP - 1	WC-03(0-5)DUP	-198	-0.0444	-	7470A	PPB	27 Jan 2018 15:06:03	U	SMPL
J1261-03MS - 1	WC-03(0-5)MS	13449	3.7315	-	7470A	PPB	27 Jan 2018 15:08:10	U	SMPL
J1261-03MSD - 1	WC-03(0-5)MSD	12957	3.5954	-	7470A	PPB	27 Jan 2018 15:10:18	U	SMPL
J1261-04 - 1	WC-04(0-5)	-159	-0.0337	-	7470A	PPB	27 Jan 2018 15:12:26	U	SMPL
J1261-05 - 1	WC-05(0-5)	-182	-0.0400	-	7470A	PPB	27 Jan 2018 15:14:34	U	SMPL
J1261-06 - 1	WC-06(5-16)	21	0.0162	-	7470A	PPB	27 Jan 2018 15:16:42	U	SMPL
CCV07 - 1	CCV07	17777	4.9290	-	7470A	PPB	27 Jan 2018 15:18:49	U	SMPL

LB92936 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 27 Jan 2018 12:19:15

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
CCB07 - 1	CCB07	-137	-0.0276		-7470A	PPB	27 Jan 2018 15:20:57	U	SMPL
J1261-07 - 1	WC-07(5-15)	-163	-0.0348		-7470A	PPB	27 Jan 2018 15:23:05	U	SMPL
J1261-08 - 1	WC-08(5-15)	268	0.0845		-7470A	PPB	27 Jan 2018 15:25:12	U	SMPL
J1261-09 - 1	WC-9(5-15)	-163	-0.0348		-7470A	PPB	27 Jan 2018 15:27:20	U	SMPL
J1261-10 - 1	WC-10(0-5)	56	0.0258		-7470A	PPB	27 Jan 2018 15:29:27	U	SMPL
J1261-11 - 1	WC-11(0-5)	-108	-0.0195		-7470A	PPB	27 Jan 2018 15:31:35	U	SMPL
J1261-12 - 1	WC-12(0-5)	-5	0.0090		-7470A	PPB	27 Jan 2018 15:33:42	U	SMPL
J1261-13 - 1	WC-13(0-5)	1100	0.3147		-7470A	PPB	27 Jan 2018 15:35:50	U	SMPL
J1261-14 - 1	WC-14(0-5)	628	0.1841		-7470A	PPB	27 Jan 2018 15:37:59	U	SMPL
J1261-15 - 1	WC-15(0-5)	776	0.2250		-7470A	PPB	27 Jan 2018 15:40:07	U	SMPL
J1261-16 - 1	WC-16(0-5)	-135	-0.0270		-7470A	PPB	27 Jan 2018 15:42:15	U	SMPL
CCV08 - 1	CCV08	17363	4.8144		-7470A	PPB	27 Jan 2018 15:44:22	U	SMPL
CCB08 - 1	CCB08	-96	-0.0162		-7470A	PPB	27 Jan 2018 15:46:30	U	SMPL
J1261-17 - 1	WC-17(0-5)	-181	-0.0397		-7470A	PPB	27 Jan 2018 15:48:39	U	SMPL
J1261-18 - 1	WC-19(5-15)	161	0.0549		-7470A	PPB	27 Jan 2018 15:50:46	U	SMPL
J1261-19 - 1	WC-20(5-15)	594	0.1747		-7470A	PPB	27 Jan 2018 15:52:54	U	SMPL
J1010-09LX5 - 1		-41	-0.0010		-7470A	PPB	27 Jan 2018 15:55:02	U	SMPL
J1010-09A - 1		14431	4.0032		-7470A	PPB	27 Jan 2018 15:57:10	U	SMPL
J1009-02LX5 - 1		-107	-0.0193		-7470A	PPB	27 Jan 2018 15:59:18	U	SMPL
J1009-02A - 1		14233	3.9484		-7470A	PPB	27 Jan 2018 16:01:25	U	SMPL
J1261-03LX5 - 1		-148	-0.0306		-7470A	PPB	27 Jan 2018 16:03:33	U	SMPL
J1261-03A - 1		14164	3.9293		-7470A	PPB	27 Jan 2018 16:05:42	U	SMPL
CCV09 - 1	CCV09	17709	4.9102		-7470A	PPB	27 Jan 2018 16:07:49	U	SMPL
CCB09 - 1	CCB09	-142	-0.0289		-7470A	PPB	27 Jan 2018 16:09:57	U	SMPL