


7470A

LB9298J
INSTRUMENT ID: CV1

Linear

 μ Abs.:

35877

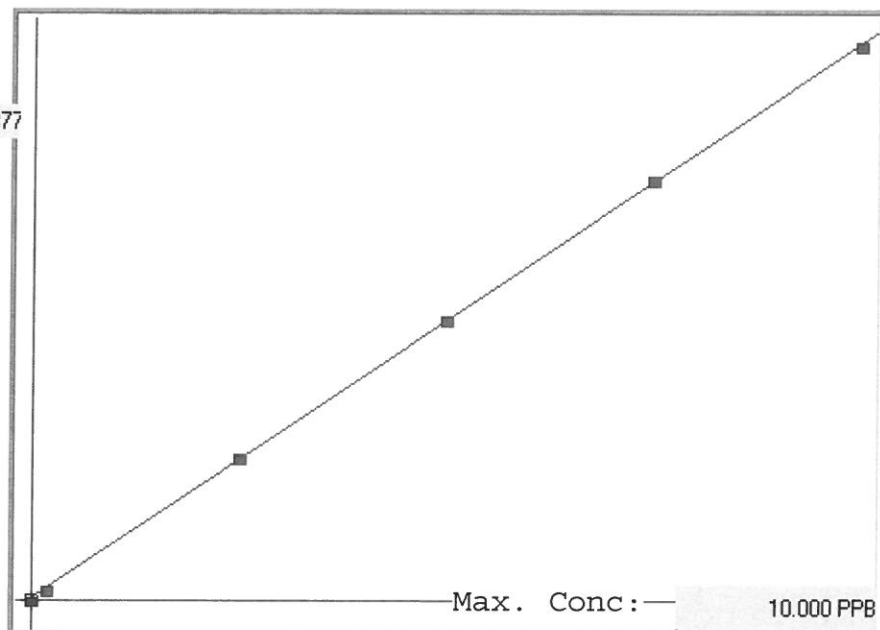

A= 0.0000e+000

B= 2.7830e-004

C= -3.4746e-002

Rho= 0.9999587

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.010	-0.010	88	0.000	88				
0.2	0.200	0.167	-0.033	725	0.0 %	725				
2.5	2.500	2.523	0.023	9190	0.0 %	9190				
5.0	5.000	5.034	0.034	18213	0.0 %	18213				
7.5	7.500	7.537	0.037	27207	0.0 %	27207				
10.0	10.000	9.950	-0.050	35877	0.0 %	35877				

LB92985 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 30 Jan 2018 10:33:47

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	88	-	0.00007470A	PPB		30 Jan 2018 10:41:54	S	Std
0.2 - 1	50.2	725	-	0.20007470A	PPB		30 Jan 2018 10:44:03	S	Std
2.5 - 1	52.5	9190	-	2.50007470A	PPB		30 Jan 2018 10:46:11	S	Std
5.0 - 1	55	18213	-	5.00007470A	PPB		30 Jan 2018 10:48:19	S	Std
7.5 - 1	57.5	27207	-	7.50007470A	PPB		30 Jan 2018 10:50:27	S	Std
10.0 - 1	510	35877	-	10.00007470A	PPB		30 Jan 2018 10:52:35	S	Std
ICV73 - 1	ICV73	14092	3.8870	-7470A	PPB		30 Jan 2018 10:55:11	U	SMPL
ICB73 - 1	ICB73	-30	-0.0431	-7470A	PPB		30 Jan 2018 10:57:17	U	SMPL
CCV26 - 1	CCV26	18301	5.0584	-7470A	PPB		30 Jan 2018 10:59:24	U	SMPL
CCB26 - 1	CCB26	-29	-0.0428	-7470A	PPB		30 Jan 2018 11:01:30	U	SMPL
CRA - 1	CRA	701	0.1603	-7470A	PPB		30 Jan 2018 11:03:38	U	SMPL
HighStd - 1	HighStd	36539	10.1339	-7470A	PPB		30 Jan 2018 11:05:44	U	SMPL
ChkStd - 1	ChkStd	24635	6.8211	-7470A	PPB		30 Jan 2018 11:07:51	U	SMPL
PB106125BL - 1	PBW	-108	-0.0648	-7470A	PPB		30 Jan 2018 11:10:00	U	SMPL
PB106125BS - 1	LCSW	13646	3.7629	-7470A	PPB		30 Jan 2018 11:12:09	U	SMPL
PB106125TB - 1	PB106092TB	-97	-0.0617	-7470A	PPB		30 Jan 2018 11:14:17	U	SMPL
J1022-11 - 1	SU-03-012618	-13	-0.0384	-7470A	PPB		30 Jan 2018 11:16:25	U	SMPL
J1022-11DUP - 1	SU-03-012618DUP	-28	-0.0425	-7470A	PPB		30 Jan 2018 11:18:33	U	SMPL
J1022-11MS - 1	SU-03-012618MS	13126	3.6182	-7470A	PPB		30 Jan 2018 11:20:42	U	SMPL
J1022-11MSD - 1	SU-03-012618MSD	13488	3.7189	-7470A	PPB		30 Jan 2018 11:22:48	U	SMPL
CCV27 - 1	CCV27	17827	4.9264	-7470A	PPB		30 Jan 2018 11:24:55	U	SMPL
CCB27 - 1	CCB27	-32	-0.0437	-7470A	PPB		30 Jan 2018 11:27:02	U	SMPL
J1338-02 - 1	OILY-STONES	37	-0.0244	-7470A	PPB		30 Jan 2018 11:29:09	U	SMPL
J1338-03 - 1	OILY-DEBRIS	5	-0.0334	-7470A	PPB		30 Jan 2018 11:31:15	U	SMPL
J1340-01 - 1	CHASSIS-WASH	-20	-0.0403	-7470A	PPB		30 Jan 2018 11:33:22	U	SMPL
J1340-02 - 1	BUS-WASH	-19	-0.0400	-7470A	PPB		30 Jan 2018 11:35:29	U	SMPL
J1341-01 - 1	CHASSIS-WASH	6	-0.0331	-7470A	PPB		30 Jan 2018 11:37:36	U	SMPL
J1341-02 - 1	BUS-WASH	31	-0.0261	-7470A	PPB		30 Jan 2018 11:39:44	U	SMPL
J1341-03 - 1	RECLAIMER-SLUDGE-PIT	48	-0.0214	-7470A	PPB		30 Jan 2018 11:41:52	U	SMPL
J1345-01 - 1	BUS-WASH	-2	-0.0353	-7470A	PPB		30 Jan 2018 11:44:00	U	SMPL
J1345-02 - 1	RECLAIMER-TANK	16	-0.0303	-7470A	PPB		30 Jan 2018 11:46:08	U	SMPL
J1345-03 - 1	ZIPPER-DRAIN	1	-0.0345	-7470A	PPB		30 Jan 2018 11:48:15	U	SMPL
CCV28 - 1	CCV28	18023	4.9810	-7470A	PPB		30 Jan 2018 11:50:22	U	SMPL
CCB28 - 1	CCB28	-17	-0.0395	-7470A	PPB		30 Jan 2018 11:52:28	U	SMPL
J1345-04 - 1	FLOOR-DRAIN	31	-0.0261	-7470A	PPB		30 Jan 2018 11:54:36	U	SMPL
J1346-04 - 1	FW-1-2	78	-0.0130	-7470A	PPB		30 Jan 2018 11:56:43	U	SMPL
J1022-11LX5 - 1		44	-0.0225	-7470A	PPB		30 Jan 2018 12:03:04	U	SMPL
J1022-11A - 1		14313	3.9485	-7470A	PPB		30 Jan 2018 12:05:10	U	SMPL
CCV29 - 1	CCV29	18265	5.0483	-7470A	PPB		30 Jan 2018 12:07:18	U	SMPL
CCB29 - 1	CCB29	-51	-0.0489	-7470A	PPB		30 Jan 2018 12:09:25	U	SMPL