


7470A

LB 93038
INSTRUMENT ID: CV1

Linear

 μ Abs.:

35462

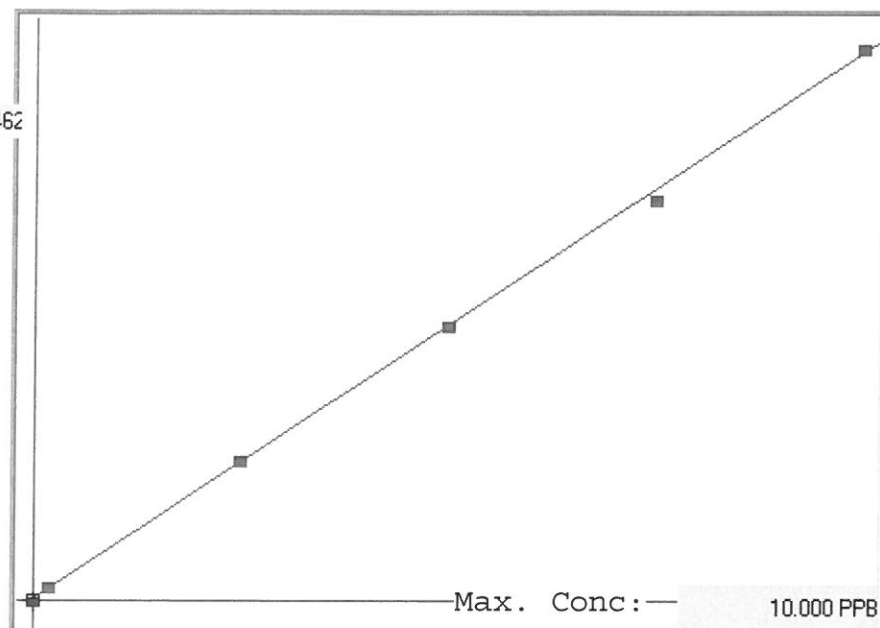

A= 0.0000e+000

B= 2.8572e-004

C= -2.3880e-002

Rho= 0.9996997

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.024	-0.024	-1	0.000	-1				
0.2	0.200	0.224	0.024	868	0.0 %	868				
2.5	2.500	2.558	0.058	9036	0.0 %	9036				
5.0	5.000	5.014	0.014	17633	0.0 %	17633				
7.5	7.500	7.319	-0.181	25701	0.0 %	25701				
10.0	10.000	10.108	0.108	35462	0.0 %	35462				

LB93038 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 01 Feb 2018 09:35:58

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50.2	-1	-	0.0000	7470A	PPB	01 Feb 2018 10:53:45	S	Std
0.2 - 1	80.2	868	-	0.2000	7470A	PPB	01 Feb 2018 10:55:54	S	Std
2.5 - 1	52.5	9036	-	2.5000	7470A	PPB	01 Feb 2018 10:58:02	S	Std
5.0 - 1	55	17633	-	5.0000	7470A	PPB	01 Feb 2018 11:00:10	S	Std
7.5 - 1	57.5	25701	-	7.5000	7470A	PPB	01 Feb 2018 11:02:18	S	Std
10.0 - 1	51.5	35462	-	10.0000	7470A	PPB	01 Feb 2018 11:04:26	S	Std
ICV78 - 1	ICV78	13183	3.7428	-	7470A	PPB	01 Feb 2018 11:07:22	U	SMPL
ICB78 - 1	ICB78	-155	-0.0682	-	7470A	PPB	01 Feb 2018 11:09:28	U	SMPL
CCV45 - 1	CCV45	18230	5.1848	-	7470A	PPB	01 Feb 2018 11:11:35	U	SMPL
CCB45 - 1	CCB45	-189	-0.0779	-	7470A	PPB	01 Feb 2018 11:13:42	U	SMPL
CRA - 1	CRA	833	0.2141	-	7470A	PPB	01 Feb 2018 11:15:49	U	SMPL
HighStd - 1	HighStd	36090	10.2878	-	7470A	PPB	01 Feb 2018 11:17:55	U	SMPL
ChkStd - 1	ChkStd	27836	7.9295	-	7470A	PPB	01 Feb 2018 11:20:02	U	SMPL
PB106240BL - 1	PBW	-245	-0.0939	-	7470A	PPB	01 Feb 2018 11:22:12	U	SMPL
PB106240BS - 1	LCSW	13965	3.9662	-	7470A	PPB	01 Feb 2018 11:24:20	U	SMPL
PB106240TB - 1	PB106202TB	-174	-0.0736	-	7470A	PPB	01 Feb 2018 11:26:28	U	SMPL
J1010-11 - 1	BU-02-013018	-84	-0.0479	-	7470A	PPB	01 Feb 2018 11:28:36	U	SMPL
J1015-21 - 1	CL-02-013018-A	-100	-0.0525	-	7470A	PPB	01 Feb 2018 11:30:44	U	SMPL
J1015-23 - 1	CL-02-013018-B	-110	-0.0553	-	7470A	PPB	01 Feb 2018 11:32:53	U	SMPL
J1015-25 - 1	CL-02-013018-C	-99	-0.0522	-	7470A	PPB	01 Feb 2018 11:34:59	U	SMPL
CCV46 - 1	CCV46	18630	5.2991	-	7470A	PPB	01 Feb 2018 11:37:06	U	SMPL
CCB46 - 1	CCB46	-179	-0.0750	-	7470A	PPB	01 Feb 2018 11:39:13	U	SMPL
J1015-25DUP - 1	CL-02-013018-CDUP	-99	-0.0522	-	7470A	PPB	01 Feb 2018 11:41:20	U	SMPL
J1015-25MS - 1	CL-02-013018-CMS	13746	3.9037	-	7470A	PPB	01 Feb 2018 11:43:27	U	SMPL
J1015-25MSD - 1	CL-02-013018-CMSD	13107	3.7211	-	7470A	PPB	01 Feb 2018 11:45:34	U	SMPL
J1015-27 - 1	CL-02-013018-D	-143	-0.0647	-	7470A	PPB	01 Feb 2018 11:47:41	U	SMPL
J1016-08 - 1	OK-03-013018	-77	-0.0459	-	7470A	PPB	01 Feb 2018 11:49:49	U	SMPL
J1023-08 - 1	TR-04-013018	-44	-0.0365	-	7470A	PPB	01 Feb 2018 11:51:56	U	SMPL
J1377-03 - 1	STONE	-48	-0.0376	-	7470A	PPB	01 Feb 2018 11:54:04	U	SMPL
J1378-02 - 1	RO-72	-15	-0.0282	-	7470A	PPB	01 Feb 2018 11:56:12	U	SMPL
J1383-03 - 1	VNJ-218	-29	-0.0322	-	7470A	PPB	01 Feb 2018 11:58:21	U	SMPL
J1383-06 - 1	SP-A	-27	-0.0316	-	7470A	PPB	01 Feb 2018 12:00:27	U	SMPL
CCV47 - 1	CCV47	18539	5.2731	-	7470A	PPB	01 Feb 2018 12:02:34	U	SMPL
CCB47 - 1	CCB47	-168	-0.0719	-	7470A	PPB	01 Feb 2018 12:04:41	U	SMPL
J1384-07 - 1	OILY-STONES-1	-42	-0.0359	-	7470A	PPB	01 Feb 2018 12:06:49	U	SMPL
J1384-13 - 1	OILY-STONES-2	-43	-0.0362	-	7470A	PPB	01 Feb 2018 12:08:56	U	SMPL
J1384-17 - 1	OILY-CONCRETE	-44	-0.0365	-	7470A	PPB	01 Feb 2018 12:11:03	U	SMPL
J1384-28 - 1	OILY-DEBRIS	-24	-0.0307	-	7470A	PPB	01 Feb 2018 12:13:10	U	SMPL
J1386-01 - 1	SOIL-CUTTINGS	-27	-0.0316	-	7470A	PPB	01 Feb 2018 12:15:17	U	SMPL
J1388-05 - 1	OILY-DEBRIS	-23	-0.0305	-	7470A	PPB	01 Feb 2018 12:17:24	U	SMPL
PB106241BL - 1	PBW	-54	-0.0393	-	7470A	PPB	01 Feb 2018 12:19:32	U	SMPL
PB106241BS - 1	LCSW	13746	3.9037	-	7470A	PPB	01 Feb 2018 12:21:41	U	SMPL
J1407-01 - 1	TW-01	-321	-0.1156	-	7470A	PPB	01 Feb 2018 12:23:49	U	SMPL
J1407-01DUP - 1	TW-01DUP	-259	-0.0979	-	7470A	PPB	01 Feb 2018 12:25:56	U	SMPL
CCV48 - 1	CCV48	18418	5.2386	-	7470A	PPB	01 Feb 2018 12:28:03	U	SMPL
CCB48 - 1	CCB48	-116	-0.0570	-	7470A	PPB	01 Feb 2018 12:30:11	U	SMPL
J1407-01MS - 1	TW-01MS	14551	4.1337	-	7470A	PPB	01 Feb 2018 12:32:19	U	SMPL
J1407-01MSD - 1	TW-01MSD	14283	4.0571	-	7470A	PPB	01 Feb 2018 12:34:26	U	SMPL
J1015-25LX5 - 1		-180	-0.0753	-	7470A	PPB	01 Feb 2018 12:36:33	U	SMPL
J1015-25A - 1		14242	4.0454	-	7470A	PPB	01 Feb 2018 12:38:40	U	SMPL
J1407-01LX5 - 1		-195	-0.0796	-	7470A	PPB	01 Feb 2018 12:40:47	U	SMPL
J1407-01A - 1		14786	4.2008	-	7470A	PPB	01 Feb 2018 12:42:55	U	SMPL
CCV49 - 1	CCV49	18214	5.1803	-	7470A	PPB	01 Feb 2018 12:45:02	U	SMPL
CCB49 - 1	CCB49	-144	-0.0650	-	7470A	PPB	01 Feb 2018 12:47:11	U	SMPL