

LB 93091


7470A

INSTRUMENT ID: CV1

Linear

 μ Abs.:

39282

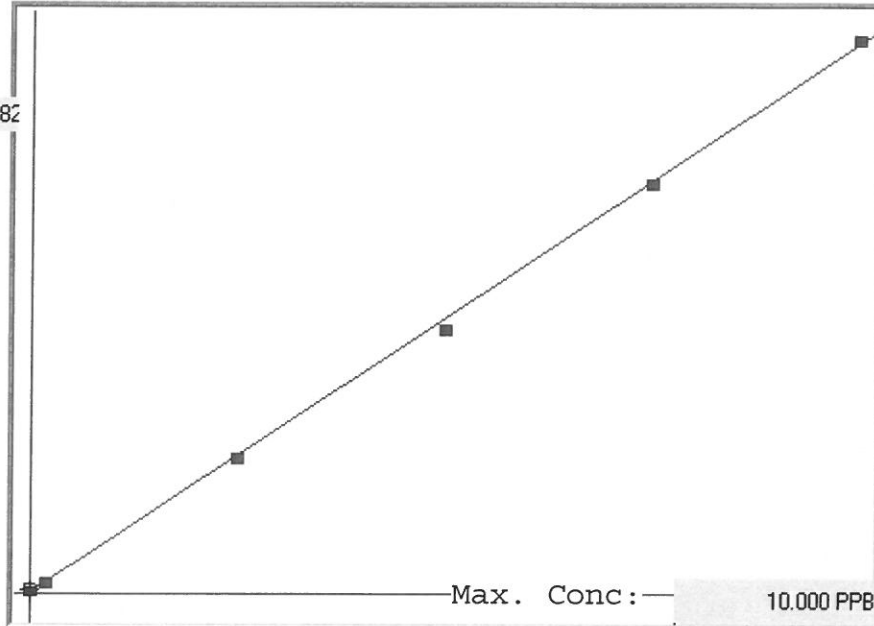

A= 0.0000e+000

B= 2.5726e-004

C= -1.4786e-002

Rho= 0.9997395

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.070	0.070	328	0.000	328				
0.2	0.200	0.225	0.025	931	0.0 %	931				
2.5	2.500	2.498	-0.002	9768	0.0 %	9768				
5.0	5.000	4.831	-0.169	18835	0.0 %	18835				
7.5	7.500	7.486	-0.014	29158	0.0 %	29158				
10.0	10.000	10.091	0.091	39282	0.0 %	39282				

LB93091 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 05 Feb 2018 12:48:59

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	328	-	0.0000	7470A	PPB	05 Feb 2018 13:09:46	S	Std
0.2 - 1	50.2	931	-	0.2000	7470A	PPB	05 Feb 2018 13:11:54	S	Std
2.5 - 1	52.5	9768	-	2.5000	7470A	PPB	05 Feb 2018 13:14:02	S	Std
5.0 - 1	55	18835	-	5.0000	7470A	PPB	05 Feb 2018 13:16:10	S	Std
7.5 - 1	57.5	29158	-	7.5000	7470A	PPB	05 Feb 2018 13:18:18	S	Std
10.0 - 1	510	39282	-	10.0000	7470A	PPB	05 Feb 2018 13:20:25	S	Std
ICV83 - 1	ICV83	15146	3.8816	-	7470A	PPB	05 Feb 2018 13:23:03	U	SMPL
ICB83 - 1	ICB83	260	0.0521	-	7470A	PPB	05 Feb 2018 13:25:09	U	SMPL
CCV67 - 1	CCV67	18955	4.8615	-	7470A	PPB	05 Feb 2018 13:27:16	U	SMPL
CCB67 - 1	CCB67	219	0.0416	-	7470A	PPB	05 Feb 2018 13:29:22	U	SMPL
CRA - 1	CRA	954	0.2306	-	7470A	PPB	05 Feb 2018 13:31:29	U	SMPL
HighStd - 1	HighStd	39236	10.0789	-	7470A	PPB	05 Feb 2018 13:33:35	U	SMPL
ChkStd - 1	ChkStd	27131	6.9648	-	7470A	PPB	05 Feb 2018 13:35:42	U	SMPL
PB106288BS - 1	LCSW	15661	4.0141	-	7470A	PPB	05 Feb 2018 13:40:00	U	SMPL
PB106288TB - 1	PB106264TB	480	0.1087	-	7470A	PPB	05 Feb 2018 13:42:08	U	SMPL
J1395-02 - 1	NB-08-020118	450	0.1010	-	7470A	PPB	05 Feb 2018 13:44:16	U	SMPL
J1423-01 - 1	CHASSIS-WASH	503	0.1146	-	7470A	PPB	05 Feb 2018 13:46:24	U	SMPL
J1429-01 - 1	CHASSIS-WASH	508	0.1159	-	7470A	PPB	05 Feb 2018 13:48:33	U	SMPL
J1429-02 - 1	BUS-WASH-COMP	566	0.1308	-	7470A	PPB	05 Feb 2018 13:50:40	U	SMPL
CCV68 - 1	CCV68	18926	4.8540	-	7470A	PPB	05 Feb 2018 13:52:46	U	SMPL
CCB68 - 1	CCB68	211	0.0395	-	7470A	PPB	05 Feb 2018 13:54:53	U	SMPL
J1429-03 - 1	RECLAIMER-SLUDGE-PIT	398	0.0876	-	7470A	PPB	05 Feb 2018 13:57:00	U	SMPL
J1431-03 - 1	132-1-PH-3	481	0.1090	-	7470A	PPB	05 Feb 2018 13:59:07	U	SMPL
J1431-06 - 1	132-1-PH-2	496	0.1128	-	7470A	PPB	05 Feb 2018 14:01:13	U	SMPL
J1431-09 - 1	132-1-PH-1	485	0.1100	-	7470A	PPB	05 Feb 2018 14:03:20	U	SMPL
J1436-04 - 1	B15	474	0.1072	-	7470A	PPB	05 Feb 2018 14:05:28	U	SMPL
J1436-08 - 1	B13	463	0.1043	-	7470A	PPB	05 Feb 2018 14:07:36	U	SMPL
J1436-12 - 1	B12	433	0.0966	-	7470A	PPB	05 Feb 2018 14:09:44	U	SMPL
J1436-16 - 1	B18	497	0.1131	-	7470A	PPB	05 Feb 2018 14:11:52	U	SMPL
J1436-20 - 1	B25	463	0.1043	-	7470A	PPB	05 Feb 2018 14:14:00	U	SMPL
J1436-20DUP - 1	B25DUP	417	0.0925	-	7470A	PPB	05 Feb 2018 14:16:07	U	SMPL
CCV69 - 1	CCV69	18946	4.8592	-	7470A	PPB	05 Feb 2018 14:18:15	U	SMPL
CCB69 - 1	CCB69	313	0.0657	-	7470A	PPB	05 Feb 2018 14:20:22	U	SMPL
J1436-20MS - 1	B25MS	14450	3.7026	-	7470A	PPB	05 Feb 2018 14:22:29	U	SMPL
J1436-20MSD - 1	B25MSD	14594	3.7396	-	7470A	PPB	05 Feb 2018 14:24:36	U	SMPL
PB106288BL - 1	PBW	366	0.0794	-	7470A	PPB	05 Feb 2018 14:26:43	U	SMPL
J1436-20LX5 - 1		407	0.0899	-	7470A	PPB	05 Feb 2018 14:28:51	U	SMPL
J1436-20A - 1		14878	3.8127	-	7470A	PPB	05 Feb 2018 14:30:58	U	SMPL
CCV70 - 1	CCV70	18842	4.8324	-	7470A	PPB	05 Feb 2018 14:33:05	U	SMPL
CCB70 - 1	CCB70	237	0.0462	-	7470A	PPB	05 Feb 2018 14:35:13	U	SMPL