

LB 93125


7470A

INSTRUMENT ID: CY2

Linear

μ Abs.:

36969

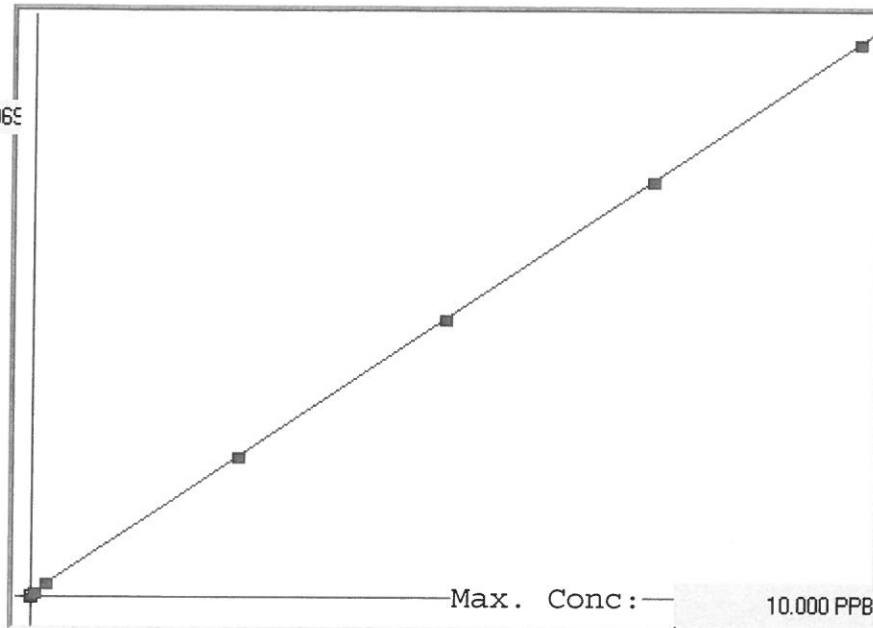

A= 0.0000e+000

B= 2.7138e-004

C= -4.2100e-002

Rho= 0.9999943

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.020	-0.020	82	0.000	82				
0.05	0.050	0.042	-0.008	310	0.0 %	310				
0.2	0.200	0.209	0.009	927	0.0 %	927				
2.5	2.500	2.516	0.016	9428	0.0 %	9428				
5.0	5.000	5.014	0.014	18630	0.0 %	18630				
7.5	7.500	7.498	-0.002	27784	0.0 %	27784				
10.0	10.000	9.990	-0.010	36969	0.0 %	36969				

LB93125 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 06 Feb 2018 15:38:29

Sample ID	Extended ID	μ Abs	Conc	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	82	-	0.0000	7470A	PPB	06 Feb 2018 15:43:57	S	Std
0.05 - 1	50.05	310	-	0.0500	7470A	PPB	06 Feb 2018 15:46:05	S	Std
0.2 - 1	50.2	927	-	0.2000	7470A	PPB	06 Feb 2018 15:48:13	S	Std
2.5 - 1	52.5	9428	-	2.5000	7470A	PPB	06 Feb 2018 15:50:21	S	Std
5.0 - 1	55	18630	-	5.0000	7470A	PPB	06 Feb 2018 15:52:29	S	Std
7.5 - 1	57.5	27784	-	7.5000	7470A	PPB	06 Feb 2018 15:54:36	S	Std
10.0 - 1	511	36969	-	10.0000	7470A	PPB	06 Feb 2018 16:01:41	S	Std
ICV86 - 1	ICV86	14335	3.8481	-	7470A	PPB	06 Feb 2018 16:04:30	U	SMPL
ICB86 - 1	ICB86	122	-0.0090	-	7470A	PPB	06 Feb 2018 16:08:59	U	SMPL
CCV81 - 1	CCV81	18147	4.8826	-	7470A	PPB	06 Feb 2018 16:11:05	U	SMPL
CCB81 - 1	CCB81	17	-0.0375	-	7470A	PPB	06 Feb 2018 16:13:11	U	SMPL
CRA - 1	CRA	933	0.2111	-	7470A	PPB	06 Feb 2018 16:15:18	U	SMPL
HighStd - 1	HighStd	36382	9.8311	-	7470A	PPB	06 Feb 2018 16:17:25	U	SMPL
ChkStd - 1	ChkStd	25340	6.8346	-	7470A	PPB	06 Feb 2018 16:19:31	U	SMPL
PB106324BL - 1	PBW	5	-0.0407	-	7470A	PPB	06 Feb 2018 16:21:40	U	SMPL
PB106324BS - 1	LCSW	13111	3.5159	-	7470A	PPB	06 Feb 2018 16:23:48	U	SMPL
PB106324TB - 1	PB106284TB	230	0.0203	-	7470A	PPB	06 Feb 2018 16:28:46	U	SMPL
J1399-02 - 1	OR-01-020218-A	26	-0.0350	-	7470A	PPB	06 Feb 2018 16:30:54	U	SMPL
J1399-02DUP - 1	OR-01-020218-ADUP	10	-0.0394	-	7470A	PPB	06 Feb 2018 16:33:02	U	SMPL
J1399-02MS - 1	OR-01-020218-AMS	13292	3.5650	-	7470A	PPB	06 Feb 2018 16:35:10	U	SMPL
J1399-02MSD - 1	OR-01-020218-AMSD	13111	3.5159	-	7470A	PPB	06 Feb 2018 16:37:16	U	SMPL
CCV82 - 1	CCV82	18090	4.8671	-	7470A	PPB	06 Feb 2018 16:39:23	U	SMPL
CCB82 - 1	CCB82	160	0.0013	-	7470A	PPB	06 Feb 2018 16:44:18	U	SMPL
J1399-04 - 1	OR-01-020218-B	21	-0.0364	-	7470A	PPB	06 Feb 2018 16:46:25	U	SMPL
J1437-03 - 1	RO-148-20	20	-0.0367	-	7470A	PPB	06 Feb 2018 16:48:31	U	SMPL
J1442-01 - 1	SECOND-FLOOR-CHASSIS-WASH	28	-0.0345	-	7470A	PPB	06 Feb 2018 16:50:38	U	SMPL
J1442-02 - 1	FIRST-FLOOR-CHASSIS-WASH	66	-0.0242	-	7470A	PPB	06 Feb 2018 16:52:46	U	SMPL
J1442-03 - 1	BUS-WASH-RECLAIM-SYSTEM	55	-0.0272	-	7470A	PPB	06 Feb 2018 16:54:53	U	SMPL
J1444-02 - 1	WC-PH3-MGP-03	29	-0.0342	-	7470A	PPB	06 Feb 2018 16:57:01	U	SMPL
J1445-03 - 1	M-4	37	-0.0321	-	7470A	PPB	06 Feb 2018 16:59:09	U	SMPL
J1453-04 - 1	P-1	31	-0.0337	-	7470A	PPB	06 Feb 2018 17:01:17	U	SMPL
J1453-08 - 1	P-2	23	-0.0359	-	7470A	PPB	06 Feb 2018 17:03:26	U	SMPL
J1453-12 - 1	P-3	51	-0.0283	-	7470A	PPB	06 Feb 2018 17:05:33	U	SMPL
CCV83 - 1	CCV83	18069	4.8614	-	7470A	PPB	06 Feb 2018 17:07:40	U	SMPL
CCB83 - 1	CCB83	104	-0.0139	-	7470A	PPB	06 Feb 2018 17:09:47	U	SMPL
PB106325BL - 1	PBW	115	-0.0109	-	7470A	PPB	06 Feb 2018 17:11:55	U	SMPL
PB106325BS - 1	LCSW	12812	3.4348	-	7470A	PPB	06 Feb 2018 17:14:02	U	SMPL
J1161-07 - 1	LOD-MDL-WATER-01-QT1-2018	255	0.0271	-	7470A	PPB	06 Feb 2018 17:16:09	U	SMPL
J1161-08 - 1	LOQ-WATER-02-QT1-2018	1782	0.4415	-	7470A	PPB	06 Feb 2018 17:18:16	U	SMPL
J1161-09 - 1	MDL-WATER-03-QT1-2018	307	0.0412	-	7470A	PPB	06 Feb 2018 17:20:24	U	SMPL
J1399-02LX5 - 1		75	-0.0217	-	7470A	PPB	06 Feb 2018 17:22:31	U	SMPL
J1399-02A - 1		14299	3.8383	-	7470A	PPB	06 Feb 2018 17:24:39	U	SMPL
CCV84 - 1	CCV84	18269	4.9157	-	7470A	PPB	06 Feb 2018 17:26:47	U	SMPL
CCB84 - 1	CCB84	37	-0.0321	-	7470A	PPB	06 Feb 2018 17:28:56	U	SMPL