

=====

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : NS

2/12/2018 9:44

Test: *Reactive*
~~Total~~ CN *Myld*

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	96.770	0.0	0.092	
ICB1	-0.327	0.0	0.004	
CCV1	242.563	0.0	0.225	
CCB1	-0.130	0.0	0.004	
PB106436BL	-0.513	0.0	0.003	
J1499-03	-0.711	0.0	0.003	
J1499-03DUP	-0.356	0.0	0.004	
J1501-02	-0.561	0.0	0.003	
J1507-03	-0.514	0.0	0.003	
J1510-06	-0.405	0.0	0.003	
J1511-04	-0.616	0.0	0.003	
J1511-05	-0.552	0.0	0.003	
J1511-06	-0.503	0.0	0.003	
J1512-03	-0.404	0.0	0.003	
CCV2	248.652	0.0	0.231	
CCB2	-0.577	0.0	0.003	
J1512-06	-1.929	0.0	0.002	
J1512-09	-0.618	0.0	0.003	
J1512-12	-0.172	0.0	0.004	
CCV3	246.537	0.0	0.229	
CCB3	-0.195	0.0	0.004	

N 21
Mean 39.307
SD 88.9864
CV% 226.39

AS

Aquakem v. 7.2AQ1

Results from time period:

Mon Feb 12 08:50:23 2018

Mon Feb 12 09:42:43 2018

Sample Id	Sam/Ctr/c/	Test short nan	Test type	Result	Result unit	Result date and time Stat
0.OPPBCN	A	Reactive CN	P	-0.6923	µg/l	2/12/2018 8:50:23
5.OPPBCN	A	Reactive CN	P	3.8407	µg/l	2/12/2018 8:50:24
10PPBCN	A	Reactive CN	P	9.4034	µg/l	2/12/2018 8:50:25
50PPBCN	A	Reactive CN	P	49.4697	µg/l	2/12/2018 8:50:26
100PPBCN	A	Reactive CN	P	102.0245	µg/l	2/12/2018 8:50:27
250PPBCN	A	Reactive CN	P	252.5646	µg/l	2/12/2018 8:50:28
500PPBCN	A	Reactive CN	P	498.3894	µg/l	2/12/2018 8:50:29
ICV1	S	Reactive CN	P	96.7697	µg/l	2/12/2018 9:34:59
ICB1	S	Reactive CN	P	-0.3268	µg/l	2/12/2018 9:35:00
CCV1	S	Reactive CN	P	242.5628	µg/l	2/12/2018 9:35:01
CCB1	S	Reactive CN	P	-0.1303	µg/l	2/12/2018 9:35:02
PB106436BL	S	Reactive CN	P	-0.5135	µg/l	2/12/2018 9:35:03
J1499-03	S	Reactive CN	P	-0.7106	µg/l	2/12/2018 9:35:04
J1499-03DUP	S	Reactive CN	P	-0.3556	µg/l	2/12/2018 9:35:05
J1501-02	S	Reactive CN	P	-0.5606	µg/l	2/12/2018 9:35:06
J1507-03	S	Reactive CN	P	-0.5135	µg/l	2/12/2018 9:35:07
J1510-06	S	Reactive CN	P	-0.4051	µg/l	2/12/2018 9:35:08
J1511-04	S	Reactive CN	P	-0.6159	µg/l	2/12/2018 9:42:33
J1511-05	S	Reactive CN	P	-0.5519	µg/l	2/12/2018 9:42:34
J1511-06	S	Reactive CN	P	-0.5032	µg/l	2/12/2018 9:42:35
J1512-03	S	Reactive CN	P	-0.4038	µg/l	2/12/2018 9:42:36
CCV2	S	Reactive CN	P	248.6517	µg/l	2/12/2018 9:42:37
CCB2	S	Reactive CN	P	-0.5772	µg/l	2/12/2018 9:42:38
J1512-06	S	Reactive CN	P	-1.9294	µg/l	2/12/2018 9:42:39
J1512-09	S	Reactive CN	P	-0.618	µg/l	2/12/2018 9:42:40
J1512-12	S	Reactive CN	P	-0.1723	µg/l	2/12/2018 9:42:41
CCV3	S	Reactive CN	P	246.5374	µg/l	2/12/2018 9:42:42
CCB3	S	Reactive CN	P	-0.1947	µg/l	2/12/2018 9:42:43

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

2/12/2018 8:57


Test Total CN

Accepted 2/12/2018 8:57

Factor 1096
Bias 0.004

Coeff. of det. 0.999923

Errors

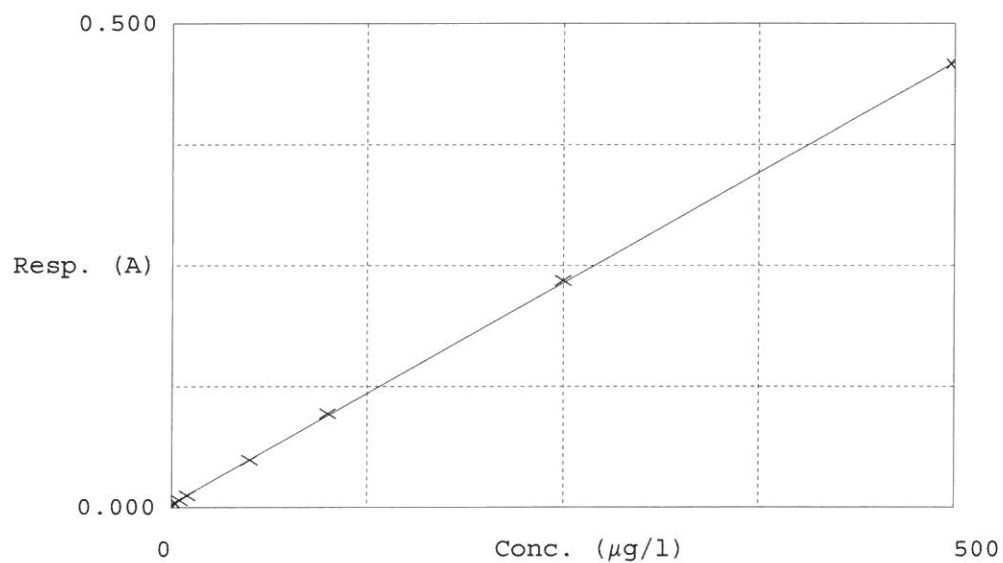

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.003	-0.6923	0.0000	
2	5.0PPBCN	0.007	3.8407	5.0000	
3	10PPBCN	0.012	9.4034	10.0000	
4	50PPBCN	0.049	49.4697	50.0000	
5	100PPBCN	0.097	102.0245	100.0000	
6	250PPBCN	0.234	252.5646	250.0000	
7	500PPBCN	0.459	498.3894	500.0000	