

2193329

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : As

2/16/2018 11:56

Test: Phenolics- mg/d

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	1.021	0.0	0.115	
ICB1	-0.002	0.0	0.009	
CCV1	1.062	0.0	0.119	
CCB1	-0.002	0.0	0.009	
PB106597BL	0.004	0.0	0.009	
PB106597BS	1.042	0.0	0.117	
J1161-01	0.014	0.0	0.010	
J1161-03	0.014	0.0	0.011	
PB106598BL	0.004	0.0	0.009	
PB106598BS	1.035	0.0	0.116	
J1161-07	0.017	0.0	0.011	
J1161-09	0.017	0.0	0.011	
CCV2	1.068	0.0	0.119	
CCB2	0.001	0.0	0.009	

N	14
Mean	0.378
SD	0.5163
CV%	136.51

As

Aquakem v. 7.2AQ1

Results from time period:

Fri Feb 16 10:53:56 2018

Fri Feb 16 11:40:39 2018

Sample Id	Sam/Ctr/c	Test short n	Test type	Result	Result unit	Result date and time	Stat
0.05PPM	A	Phenolics-	P	0.0518	mg/l	2/16/2018 10:53:56	
0.1PPM	A	Phenolics-	P	0.1029	mg/l	2/16/2018 10:53:57	
0.25PPM	A	Phenolics-	P	0.2501	mg/l	2/16/2018 10:53:58	
0.50PPM	A	Phenolics-	P	0.4974	mg/l	2/16/2018 10:53:59	
1.0PPM	A	Phenolics-	P	0.9946	mg/l	2/16/2018 10:54:00	
2.0PPM	A	Phenolics-	P	2.0031	mg/l	2/16/2018 10:54:01	
ICV1	S	Phenolics-	P	1.0207	mg/l	2/16/2018 11:20:54	
ICB1	S	Phenolics-	P	-0.0015	mg/l	2/16/2018 11:20:55	
CCV1	S	Phenolics-	P	1.062	mg/l	2/16/2018 11:20:56	
CCB1	S	Phenolics-	P	-0.0018	mg/l	2/16/2018 11:20:57	
PB106597BL	S	Phenolics-	P	0.004	mg/l	2/16/2018 11:40:30	
PB106597BS	S	Phenolics-	P	1.0417	mg/l	2/16/2018 11:40:31	
J1161-01	S	Phenolics-	P	0.0136	mg/l	2/16/2018 11:40:32	
J1161-03	S	Phenolics-	P	0.0143	mg/l	2/16/2018 11:40:33	
PB106598BL	S	Phenolics-	P	0.0042	mg/l	2/16/2018 11:40:34	
PB106598BS	S	Phenolics-	P	1.0351	mg/l	2/16/2018 11:40:35	
J1161-07	S	Phenolics-	P	0.0165	mg/l	2/16/2018 11:40:36	
J1161-09	S	Phenolics-	P	0.0172	mg/l	2/16/2018 11:40:37	
CCV2	S	Phenolics-	P	1.0677	mg/l	2/16/2018 11:40:38	
CCB2	S	Phenolics-	P	0.0008	mg/l	2/16/2018 11:40:39	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

2/16/2018 11:02


Test Phenolics-

Accepted 2/16/2018 11:02

Factor 9.671
Bias 0.009

Coeff. of det. 0.999980

Errors

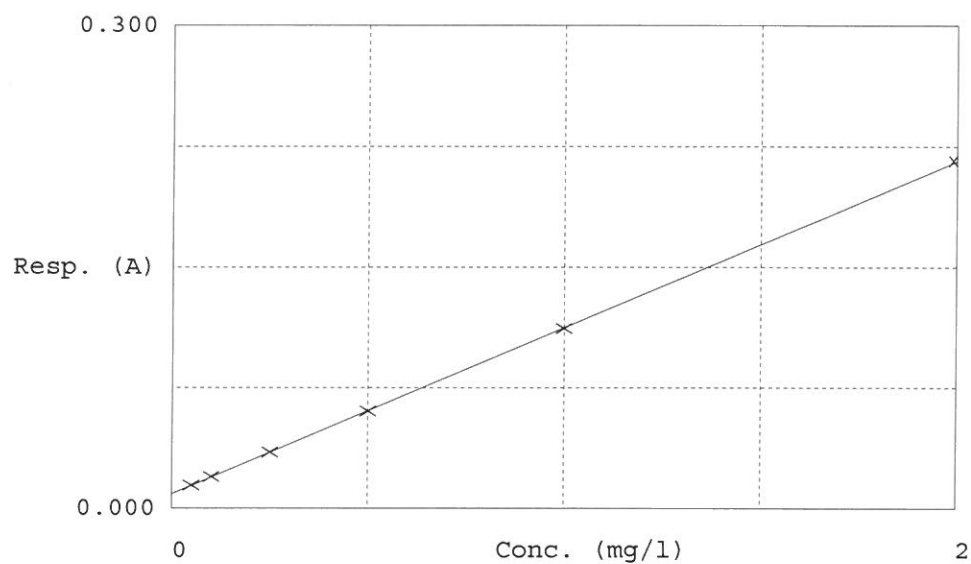

	Calibrator	Response	Calc. con.	Conc.	Errors
1	Phenol-2	0.014	0.0518	0.0500	
2	Phenol-2	0.020	0.1029	0.1000	
3	Phenol-2	0.035	0.2501	0.2500	
4	Phenol-2	0.060	0.4974	0.5000	
5	Phenol-2	0.112	0.9946	1.0000	
6	Phenol-2	0.216	2.0031	2.0000	