

L393578


245.1

INSTRUMENT ID: CV2

Linear

μ Abs.:

34265

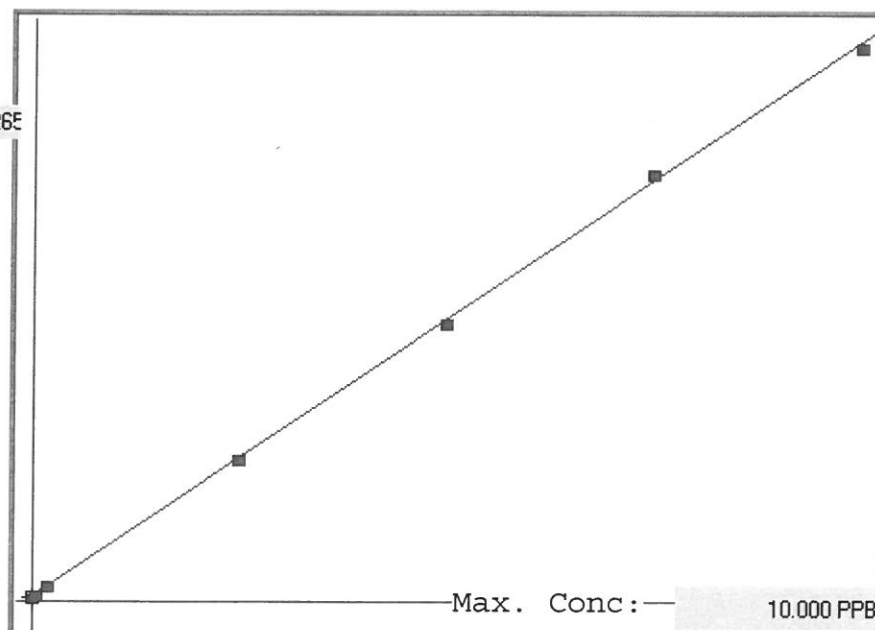

A= 0.0000e+000

B= 2.9150e-004

C= -8.2343e-002

Rho= 0.9998100

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.006	-0.006	263	0.000	263				
0.05	0.050	0.046	-0.004	441	0.0 %	441				
0.2	0.200	0.203	0.003	978	0.0 %	978				
2.5	2.500	2.497	-0.003	8850	0.0 %	8850				
5.0	5.000	4.946	-0.054	17250	0.0 %	17250				
7.5	7.500	7.658	0.158	26552	0.0 %	26552				
10.0	10.000	9.906	-0.094	34265	0.0 %	34265				

LB93578 INSTRUMENT ID : CV1

Method: 245.1

Operator: Admin

Date of Analysis: 28 Feb 2018 12:43:05

Sample ID	Extended ID	µ Abs.	Conc.	Std Cond	Method	Units	Date	Type	Type
0.0 - 1	50	263	-	0.0000	245.1	PPB	28 Feb 2018 12:48:59	S	Std
0.05 - 1	50.05	441	-	0.0500	245.1	PPB	28 Feb 2018 12:51:07	S	Std
0.2 - 1	50.2	978	-	0.2000	245.1	PPB	28 Feb 2018 12:53:15	S	Std
2.5 - 1	52.5	8850	-	2.5000	245.1	PPB	28 Feb 2018 12:55:23	S	Std
5.0 - 1	55	17250	-	5.0000	245.1	PPB	28 Feb 2018 12:57:31	S	Std
7.5 - 1	57.5	26552	-	7.5000	245.1	PPB	28 Feb 2018 12:59:38	S	Std
10.0 - 1	510	34265	-	10.0000	245.1	PPB	28 Feb 2018 13:01:46	S	Std
ICV21 - 1	ICV21	13401	3.8240	-245.1		PPB	28 Feb 2018 13:04:40	U	SMPL
ICB21 - 1	ICB21	61	-0.0646	-245.1		PPB	28 Feb 2018 13:06:46	U	SMPL
CCV42 - 1	CCV42	18180	5.2171	-245.1		PPB	28 Feb 2018 13:08:53	U	SMPL
CCB42 - 1	CCB42	50	-0.0678	-245.1		PPB	28 Feb 2018 13:10:59	U	SMPL
CRA - 1	CRA	472	0.0552	-245.1		PPB	28 Feb 2018 13:21:14	U	SMPL
HighStd - 1	HighStd	34821	10.0679	-245.1		PPB	28 Feb 2018 13:23:20	U	SMPL
ChkStd - 1	ChkStd	24629	7.0970	-245.1		PPB	28 Feb 2018 13:25:27	U	SMPL
PB106896BL - 1	PBW	-184	-0.1360	-245.1		PPB	28 Feb 2018 13:27:36	U	SMPL
PB106896BS - 1	LCSW	13598	3.8814	-245.1		PPB	28 Feb 2018 13:29:44	U	SMPL
J1641-01 - 1	EFFLUENT-DAY1-METALS	339	0.0165	-245.1		PPB	28 Feb 2018 13:31:52	U	SMPL
J1641-01DUP - 1	EFFLUENT-DAY1-METALSDUP	19	-0.0768	-245.1		PPB	28 Feb 2018 13:34:00	U	SMPL
J1641-01MS - 1	EFFLUENT-DAY1-METALSMS	13057	3.7237	-245.1		PPB	28 Feb 2018 13:36:09	U	SMPL
J1641-01MSD - 1	EFFLUENT-DAY1-METALSMDS	12049	3.4299	-245.1		PPB	28 Feb 2018 13:38:17	U	SMPL
J1693-01 - 1	22-52W-ZN5-KITCHENSINK	-211	-0.1438	-245.1		PPB	28 Feb 2018 13:40:24	U	SMPL
CCV43 - 1	CCV43	16631	4.7656	-245.1		PPB	28 Feb 2018 13:42:31	U	SMPL
CCB43 - 1	CCB43	21	-0.0762	-245.1		PPB	28 Feb 2018 13:44:37	U	SMPL
J1693-02 - 1	23-52W-ZN5-MBBTHSHWR	-123	-0.1182	-245.1		PPB	28 Feb 2018 13:46:44	U	SMPL
J1693-03 - 1	24-52E-ZN5-KITCHENSINK	-145	-0.1246	-245.1		PPB	28 Feb 2018 13:48:51	U	SMPL
J1693-04 - 1	25-52E-ZN5-MBBTHSHWR	-149	-0.1258	-245.1		PPB	28 Feb 2018 13:50:57	U	SMPL
J1693-05 - 1	26-PENTHOUSE53-ZN5-KITCHENSINK	-136	-0.1220	-245.1		PPB	28 Feb 2018 13:53:04	U	SMPL
J1693-06 - 1	27-PENTHOUSE53-ZN5-MBBTHSHWR	-161	-0.1293	-245.1		PPB	28 Feb 2018 13:55:12	U	SMPL
PB106897BL - 1	PBW	57	-0.0657	-245.1		PPB	28 Feb 2018 13:59:28	U	SMPL
PB106897BS - 1	LCSW	12322	3.5095	-245.1		PPB	28 Feb 2018 14:01:36	U	SMPL
J1692-01 - 1	1-BSMT-CITY-WATER	-231	-0.1497	-245.1		PPB	28 Feb 2018 14:03:44	U	SMPL
J1692-02 - 1	2-EQUIPMENT-BLANK	-118	-0.1167	-245.1		PPB	28 Feb 2018 14:05:51	U	SMPL
CCV44 - 1	CCV44	17006	4.8749	-245.1		PPB	28 Feb 2018 14:07:58	U	SMPL
CCB44 - 1	CCB44	31	-0.0733	-245.1		PPB	28 Feb 2018 14:10:04	U	SMPL
J1692-03 - 1	3-16BE-ZN-2-KITCHENSINK	-126	-0.1191	-245.1		PPB	28 Feb 2018 14:12:12	U	SMPL
J1692-04 - 1	4-16BE-ZN-2-MBBTHSHWR	-120	-0.1173	-245.1		PPB	28 Feb 2018 14:14:19	U	SMPL
J1692-05 - 1	5-18AW-ZN-2-KITCHENSINK	-100	-0.1115	-245.1		PPB	28 Feb 2018 14:16:26	U	SMPL
J1692-06 - 1	6-18AW-ZN-2-MBBTHSHWR	-105	-0.1129	-245.1		PPB	28 Feb 2018 14:18:33	U	SMPL
J1692-07 - 1	7-15AE-ZN-2-KITCHENSINK	-107	-0.1135	-245.1		PPB	28 Feb 2018 14:20:41	U	SMPL
J1692-08 - 1	8-15AE-ZN-2-MBBTHSHWR	-111	-0.1147	-245.1		PPB	28 Feb 2018 14:22:48	U	SMPL
J1692-09 - 1	9-15AW-ZN-2-KITCHENSINK	-128	-0.1197	-245.1		PPB	28 Feb 2018 14:24:56	U	SMPL
J1692-10 - 1	10-15AW-ZN-2-MBBTHSHWR	-119	-0.1170	-245.1		PPB	28 Feb 2018 14:27:05	U	SMPL
J1692-11 - 1	11-14AW-ZN-2-KITCHENSINK	-177	-0.1339	-245.1		PPB	28 Feb 2018 14:29:13	U	SMPL
J1692-12 - 1	12-14AW-ZN-2-MBBTHSHWR	-129	-0.1199	-245.1		PPB	28 Feb 2018 14:31:20	U	SMPL
CCV45 - 1	CCV45	16284	4.6644	-245.1		PPB	28 Feb 2018 14:33:27	U	SMPL
CCB45 - 1	CCB45	67	-0.0628	-245.1		PPB	28 Feb 2018 14:35:34	U	SMPL
J1692-13 - 1	13-17AW-ZN-2-KITCHENSINK	-161	-0.1293	-245.1		PPB	28 Feb 2018 14:37:43	U	SMPL
J1692-14 - 1	14-17AW-ZN-2-MBBTHSHWR	-84	-0.1068	-245.1		PPB	28 Feb 2018 14:39:50	U	SMPL
J1692-15 - 1	15-47E-ZN-5-KITCHENSINK	-71	-0.1030	-245.1		PPB	28 Feb 2018 14:41:57	U	SMPL
J1692-16 - 1	16-47E-ZN-5-MBBTHSHWR	-83	-0.1065	-245.1		PPB	28 Feb 2018 14:44:04	U	SMPL
J1692-17 - 1	17-46E-ZN-5-KITCHENSINK	-157	-0.1281	-245.1		PPB	28 Feb 2018 14:46:11	U	SMPL
J1692-18 - 1	18-46E-ZN-5-MBBTHSHWR	-148	-0.1255	-245.1		PPB	28 Feb 2018 14:48:18	U	SMPL
J1692-19 - 1	20-45W-ZN-5-KITCHENSINK	-148	-0.1255	-245.1		PPB	28 Feb 2018 14:50:27	U	SMPL
J1692-20 - 1	21-45W-ZN-5-MBBTHSHWR	-163	-0.1299	-245.1		PPB	28 Feb 2018 14:52:35	U	SMPL
J1692-20DUP - 1	21-45W-ZN-5-MBBTHSHWRDUP	-114	-0.1156	-245.1		PPB	28 Feb 2018 14:54:44	U	SMPL
J1692-20MS - 1	21-45W-ZN-5-MBBTHSHWRMS	12303	3.5040	-245.1		PPB	28 Feb 2018 14:56:51	U	SMPL
CCV46 - 1	CCV46	17043	4.8857	-245.1		PPB	28 Feb 2018 14:58:58	U	SMPL
CCB46 - 1	CCB46	-12	-0.0858	-245.1		PPB	28 Feb 2018 15:01:06	U	SMPL
J1692-20MSD - 1	21-45W-ZN-5-MBBTHSHWRMSD	12088	3.4413	-245.1		PPB	28 Feb 2018 15:03:15	U	SMPL
J1641-01LX5 - 1		397	0.0334	-245.1		PPB	28 Feb 2018 15:05:22	U	SMPL
J1641-01A - 1		12715	3.6240	-245.1		PPB	28 Feb 2018 15:07:30	U	SMPL
J1692-20LX5 - 1		47	-0.0686	-245.1		PPB	28 Feb 2018 15:09:37	U	SMPL
J1692-20A - 1		12825	3.6561	-245.1		PPB	28 Feb 2018 15:11:45	U	SMPL
CCV47 - 1	CCV47	16584	4.7519	-245.1		PPB	28 Feb 2018 15:13:53	U	SMPL
CCB47 - 1	CCB47	-7	-0.0844	-245.1		PPB	28 Feb 2018 15:16:02	U	SMPL