


7470A

LB 93712
INSTRUMENT ID: CV2

Linear

 μ Abs.:

34235

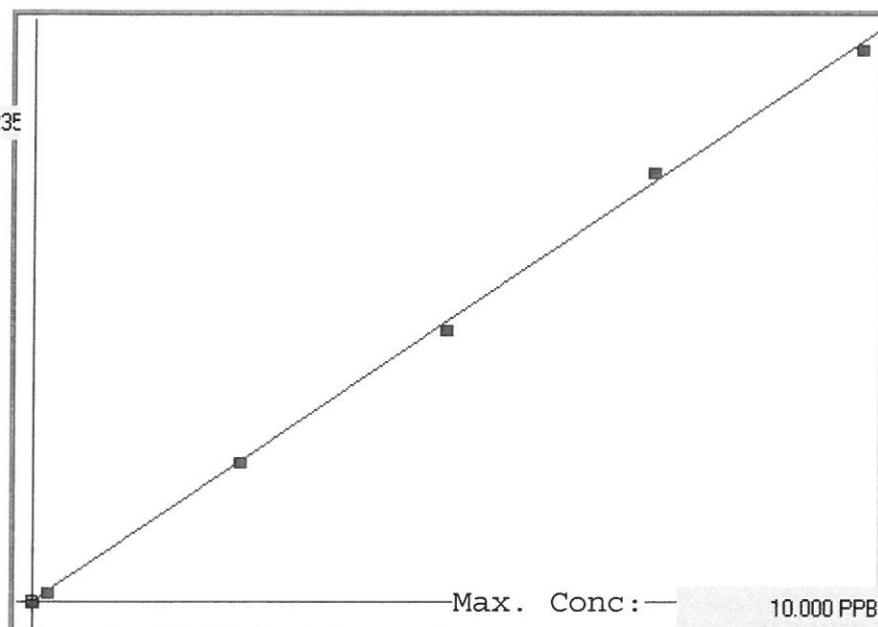

A= 0.0000e+000

B= 2.8874e-004

C= 1.9380e-003

Rho= 0.9996171

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.023	-0.023	-85	0.000	-85				
0.2	0.200	0.208	0.008	712	0.0 %	712				
2.5	2.500	2.528	0.028	8747	0.0 %	8747				
5.0	5.000	4.903	-0.097	16973	0.0 %	16973				
7.5	7.500	7.698	0.198	26652	0.0 %	26652				
10.0	10.000	9.887	-0.113	34235	0.0 %	34235				

LB93712 INSTRUMENT ID : CV1

Method: 7470A		Operator: Admin		Date of Analysis: 06 Mar 2018 10:34:49				
Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type
0.0 - 1	30	-85	-	0.0000	7470A	PPB	06 Mar 2018 10:46:38	S Std
0.2 - 1	30.2	712	-	0.2000	7470A	PPB	06 Mar 2018 10:48:46	S Std
2.5 - 1	32.5	8747	-	2.5000	7470A	PPB	06 Mar 2018 10:50:54	S Std
5.0 - 1	35	16973	-	5.0000	7470A	PPB	06 Mar 2018 10:53:02	S Std
7.5 - 1	37.5	26652	-	7.5000	7470A	PPB	06 Mar 2018 10:55:10	S Std
10.0 - 1	310	34235	-	10.0000	7470A	PPB	06 Mar 2018 10:59:55	S Std
ICV30 - 1	ICV30	13976	4.0374	-	7470A	PPB	06 Mar 2018 11:02:53	U SMPL
ICB30 - 1	ICB30	-283	-0.0798	-	7470A	PPB	06 Mar 2018 11:04:59	U SMPL
CCV95 - 1	CCV95	18278	5.2796	-	7470A	PPB	06 Mar 2018 11:07:06	U SMPL
CCB95 - 1	CCB95	-305	-0.0861	-	7470A	PPB	06 Mar 2018 11:09:13	U SMPL
CRA - 1	CRA	682	0.1989	-	7470A	PPB	06 Mar 2018 11:11:20	U SMPL
HighStd - 1	HighStd	34882	10.0739	-	7470A	PPB	06 Mar 2018 11:13:27	U SMPL
ChkStd - 1	ChkStd	24209	6.9922	-	7470A	PPB	06 Mar 2018 11:15:34	U SMPL
PB107096BL - 1	PBW	-139	-0.0382	-	7470A	PPB	06 Mar 2018 11:20:24	U SMPL
PB107096BS - 1	LCSW	12729	3.6774	-	7470A	PPB	06 Mar 2018 11:22:31	U SMPL
PB107096TB - 1	PB107041TB	-202	-0.0564	-	7470A	PPB	06 Mar 2018 11:24:39	U SMPL
J1761-02 - 1	TR-04-0302018	-84	-0.0223	-	7470A	PPB	06 Mar 2018 11:26:47	U SMPL
J1761-02DUP - 1	TR-04-0302018DUP	-81	-0.0215	-	7470A	PPB	06 Mar 2018 11:28:55	U SMPL
J1761-02MS - 1	TR-04-0302018MS	12982	3.7504	-	7470A	PPB	06 Mar 2018 11:31:04	U SMPL
J1761-02MSD - 1	TR-04-0302018MSD	13253	3.8287	-	7470A	PPB	06 Mar 2018 11:33:11	U SMPL
CCV96 - 1	CCV96	17648	5.0977	-	7470A	PPB	06 Mar 2018 11:35:18	U SMPL
CCB96 - 1	CCB96	-304	-0.0858	-	7470A	PPB	06 Mar 2018 11:37:25	U SMPL
J1783-04 - 1	SLUDGE	55	0.0178	-	7470A	PPB	06 Mar 2018 11:39:32	U SMPL
J1786-05 - 1	SAMPLE-1-24+31-WEST	-128	-0.0350	-	7470A	PPB	06 Mar 2018 11:41:39	U SMPL
J1786-06 - 1	SAMPLE-2-25+71-WEST	-124	-0.0339	-	7470A	PPB	06 Mar 2018 11:43:45	U SMPL
J1792-02 - 1	TP-6	-82	-0.0217	-	7470A	PPB	06 Mar 2018 11:45:52	U SMPL
J1792-04 - 1	TP-7	-74	-0.0194	-	7470A	PPB	06 Mar 2018 11:47:59	U SMPL
J1792-06 - 1	TP-8	38	0.0129	-	7470A	PPB	06 Mar 2018 11:50:07	U SMPL
J1792-08 - 1	TP-12	-51	-0.0128	-	7470A	PPB	06 Mar 2018 11:52:15	U SMPL
J1792-10 - 1	TP-13	-48	-0.0119	-	7470A	PPB	06 Mar 2018 11:54:23	U SMPL
PB107097BL - 1	PBW	-67	-0.0174	-	7470A	PPB	06 Mar 2018 11:56:31	U SMPL
PB107097BS - 1	LCSW	12342	3.5656	-	7470A	PPB	06 Mar 2018 11:58:38	U SMPL
CCV97 - 1	CCV97	17081	4.9340	-	7470A	PPB	06 Mar 2018 12:00:45	U SMPL
CCB97 - 1	CCB97	-294	-0.0830	-	7470A	PPB	06 Mar 2018 12:02:52	U SMPL
PB107097TB - 1	PB107043TB	-98	-0.0264	-	7470A	PPB	06 Mar 2018 12:05:00	U SMPL
J1792-12 - 1	TP-7	-65	-0.0168	-	7470A	PPB	06 Mar 2018 12:07:07	U SMPL
J1792-12DUP - 1	TP-7DUP	-54	-0.0137	-	7470A	PPB	06 Mar 2018 12:09:14	U SMPL
J1792-12MS - 1	TP-7MS	12777	3.6912	-	7470A	PPB	06 Mar 2018 12:11:21	U SMPL
J1792-12MSD - 1	TP-7MSD	12701	3.6693	-	7470A	PPB	06 Mar 2018 12:13:28	U SMPL
J1792-14 - 1	TP-8	-192	-0.0535	-	7470A	PPB	06 Mar 2018 12:15:36	U SMPL
J1792-16 - 1	TP-13	-98	-0.0264	-	7470A	PPB	06 Mar 2018 12:17:45	U SMPL
PB107099BL - 1	PBW	-66	-0.0171	-	7470A	PPB	06 Mar 2018 12:19:53	U SMPL
PB107099BS - 1	LCSW	12632	3.6494	-	7470A	PPB	06 Mar 2018 12:22:01	U SMPL
J1779-08 - 1	DRUM-1-4	-274	-0.0772	-	7470A	PPB	06 Mar 2018 12:24:08	U SMPL
CCV98 - 1	CCV98	17506	5.0567	-	7470A	PPB	06 Mar 2018 12:26:16	U SMPL
CCB98 - 1	CCB98	-299	-0.0844	-	7470A	PPB	06 Mar 2018 12:28:23	U SMPL
J1792-11 - 1	TP-7	-150	-0.0414	-	7470A	PPB	06 Mar 2018 12:30:31	U SMPL
J1792-11DUP - 1	TP-7DUP	-135	-0.0370	-	7470A	PPB	06 Mar 2018 12:32:38	U SMPL
J1792-11MS - 1	TP-7MS	15103	4.3629	-	7470A	PPB	06 Mar 2018 12:34:46	U SMPL
J1792-11MSD - 1	TP-7MSD	15020	4.3389	-	7470A	PPB	06 Mar 2018 12:36:53	U SMPL
J1792-13 - 1	TP-8	-224	-0.0627	-	7470A	PPB	06 Mar 2018 12:39:01	U SMPL
J1792-15 - 1	TP-13	-162	-0.0448	-	7470A	PPB	06 Mar 2018 12:41:08	U SMPL
CCV99 - 1	CCV99	17648	5.0977	-	7470A	PPB	06 Mar 2018 12:43:16	U SMPL
CCB99 - 1	CCB99	-281	-0.0792	-	7470A	PPB	06 Mar 2018 12:45:24	U SMPL
J1761-02LX5 - 1		-138	-0.0379	-	7470A	PPB	06 Mar 2018 12:47:34	U SMPL
J1761-02A - 1		13307	3.8443	-	7470A	PPB	06 Mar 2018 12:49:41	U SMPL
J1792-12LX5 - 1		-225	-0.0630	-	7470A	PPB	06 Mar 2018 12:51:48	U SMPL
J1792-12A - 1		13629	3.9372	-	7470A	PPB	06 Mar 2018 12:53:55	U SMPL
J1792-11LX5 - 1		-234	-0.0656	-	7470A	PPB	06 Mar 2018 12:56:02	U SMPL
J1792-11A - 1		15099	4.3617	-	7470A	PPB	06 Mar 2018 12:58:10	U SMPL
CCV01 - 1	CCV01	17543	5.0674	-	7470A	PPB	06 Mar 2018 13:00:17	U SMPL
CCB01 - 1	CCB01	-293	-0.0827	-	7470A	PPB	06 Mar 2018 13:02:24	U SMPL