

LB93823


7470A

INSTRUMENT ID: CV2

Linear

μ Abs.:

34700

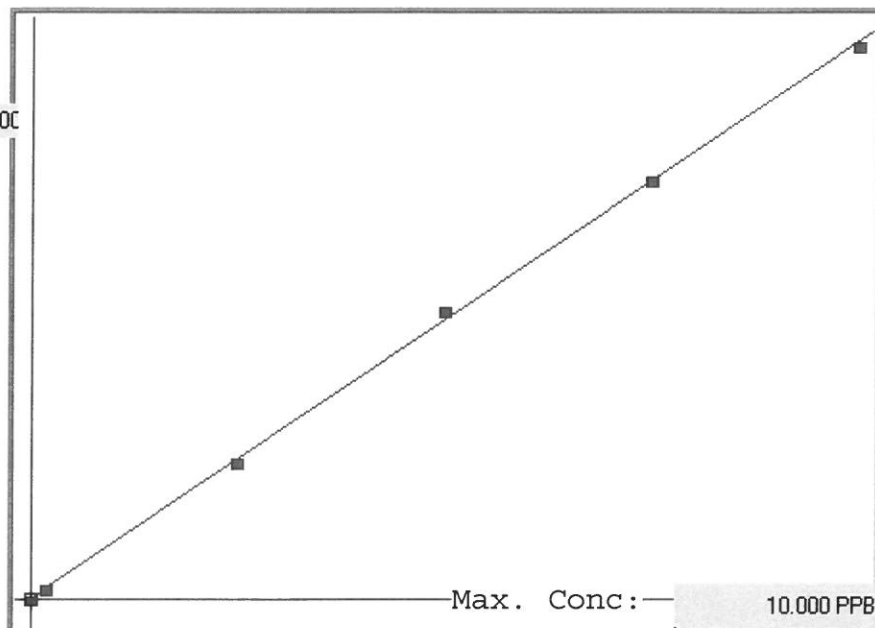

A= 0.0000e+000

B= 2.8657e-004

C= -9.8868e-003

Rho= 0.9997995

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.016	-0.016	-22	0.000	-22				
0.2	0.200	0.188	-0.012	689	0.0 %	689				
2.5	2.500	2.438	-0.062	8543	0.0 %	8543				
5.0	5.000	5.156	0.156	18025	0.0 %	18025				
7.5	7.500	7.501	0.001	26209	0.0 %	26209				
10.0	10.000	9.934	-0.066	34700	0.0 %	34700				

LB93823 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 12 Mar 2018 11:10:39

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-22	-	0.0000	7470A	PPB	12 Mar 2018 11:17:26	S	Std
0.2 - 1	50.2	689	-	0.2000	7470A	PPB	12 Mar 2018 11:19:34	S	Std
2.5 - 1	52.5	8543	-	2.5000	7470A	PPB	12 Mar 2018 11:21:43	S	Std
5.0 - 1	55	18025	-	5.0000	7470A	PPB	12 Mar 2018 11:23:51	S	Std
7.5 - 1	57.5	26209	-	7.5000	7470A	PPB	12 Mar 2018 11:25:59	S	Std
10.0 - 1	510	34700	-	10.0000	7470A	PPB	12 Mar 2018 11:28:07	S	Std
ICV38 - 1	ICV38	14412	4.1201	-	7470A	PPB	12 Mar 2018 11:30:51	U	SMPL
ICB38 - 1	ICB38	-182	-0.0620	-	7470A	PPB	12 Mar 2018 11:32:57	U	SMPL
CCV36 - 1	CCV36	18458	5.2796	-	7470A	PPB	12 Mar 2018 11:35:04	U	SMPL
CCB36 - 1	CCB36	-217	-0.0721	-	7470A	PPB	12 Mar 2018 11:37:11	U	SMPL
CRA - 1	CRA	681	0.1853	-	7470A	PPB	12 Mar 2018 11:39:18	U	SMPL
HighStd - 1	HighStd	35409	10.1372	-	7470A	PPB	12 Mar 2018 11:41:25	U	SMPL
ChkStd - 1	ChkStd	24825	7.1042	-	7470A	PPB	12 Mar 2018 11:43:31	U	SMPL
PB107225BL - 1	PBW	-255	-0.0830	-	7470A	PPB	12 Mar 2018 11:45:41	U	SMPL
PB107225BS - 1	LCSW	13889	3.9703	-	7470A	PPB	12 Mar 2018 11:47:50	U	SMPL
PB107225TB - 1	PB107187TB	-145	-0.0514	-	7470A	PPB	12 Mar 2018 11:49:57	U	SMPL
J1755-02 - 1	OK-03-030818	-54	-0.0254	-	7470A	PPB	12 Mar 2018 11:52:06	U	SMPL
J1853-02 - 1	TP1-WC	-42	-0.0219	-	7470A	PPB	12 Mar 2018 11:54:14	U	SMPL
J1855-04 - 1	TP-6-COMP	12	-0.0064	-	7470A	PPB	12 Mar 2018 11:56:23	U	SMPL
J1855-07 - 1	TP-7-A-COMP	-21	-0.0159	-	7470A	PPB	12 Mar 2018 11:58:29	U	SMPL
CCV37 - 1	CCV37	18312	5.2378	-	7470A	PPB	12 Mar 2018 12:00:36	U	SMPL
CCB37 - 1	CCB37	-199	-0.0669	-	7470A	PPB	12 Mar 2018 12:02:43	U	SMPL
J1855-10 - 1	TP-7-B-COMP	-37	-0.0205	-	7470A	PPB	12 Mar 2018 12:04:50	U	SMPL
J1855-14 - 1	TP-4-COMP	-22	-0.0162	-	7470A	PPB	12 Mar 2018 12:06:57	U	SMPL
J1855-14DUP - 1	TP-4-COMP DUP	1	-0.0096	-	7470A	PPB	12 Mar 2018 12:09:04	U	SMPL
J1855-14MS - 1	TP-4-COMPMS	13082	3.7390	-	7470A	PPB	12 Mar 2018 12:11:11	U	SMPL
J1855-14MSD - 1	TP-4-COMPMSD	13545	3.8717	-	7470A	PPB	12 Mar 2018 12:13:19	U	SMPL
J1855-14LX5 - 1		-158	-0.0552	-	7470A	PPB	12 Mar 2018 12:15:26	U	SMPL
J1855-14A - 1		14823	4.2379	-	7470A	PPB	12 Mar 2018 12:17:34	U	SMPL
CCV38 - 1	CCV38	18120	5.1827	-	7470A	PPB	12 Mar 2018 12:19:43	U	SMPL
CCB38 - 1	CCB38	-176	-0.0603	-	7470A	PPB	12 Mar 2018 12:21:51	U	SMPL