

245.1


LB93868

INSTRUMENT ID: CV1

Linear

 μ Abs.:

37017

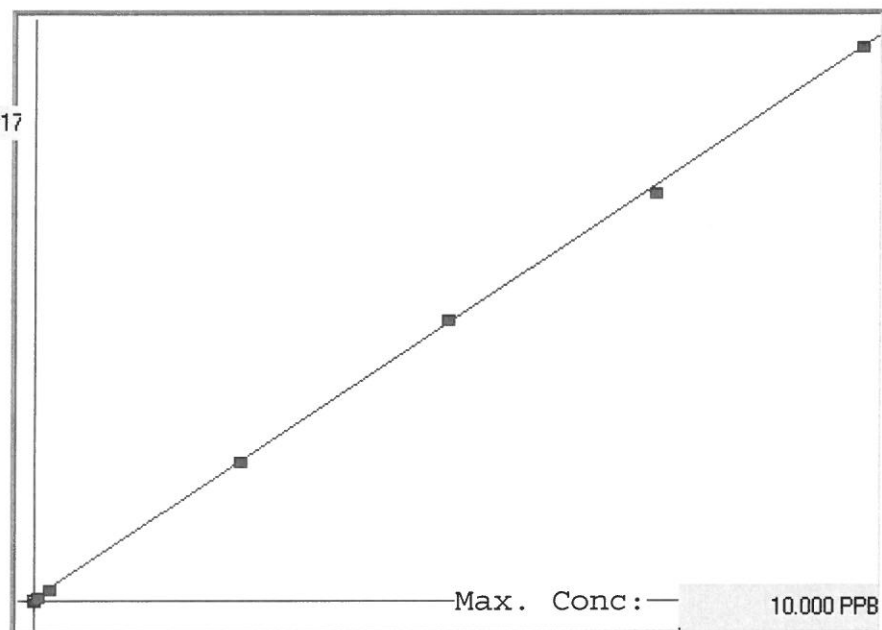

A= 0.0000e+000

B= 2.7180e-004

C= -3.8832e-002

Rho= 0.9998766

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.036	-0.036	11	0.000	11				
0.05	0.050	0.052	0.002	336	0.0 %	336				
0.2	0.200	0.203	0.003	888	0.0 %	888				
2.5	2.500	2.510	0.010	9379	0.0 %	9379				
5.0	5.000	5.104	0.104	18921	0.0 %	18921				
7.5	7.500	7.394	-0.106	27349	0.0 %	27349				
10.0	10.000	10.022	0.022	37017	0.0 %	37017				

LB93868 INSTRUMENT ID : CV1

Method: 245.1

Operator: Admin

Date of Analysis: 13 Mar 2018 14:27:19

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	11	-	0.0000	245.1	PPB	13 Mar 2018 14:30:39	S	Std
0.05 - 1	50.05	336	-	0.0500	245.1	PPB	13 Mar 2018 14:32:47	S	Std
0.2 - 1	50.2	888	-	0.2000	245.1	PPB	13 Mar 2018 14:34:56	S	Std
2.5 - 1	52.5	9379	-	2.5000	245.1	PPB	13 Mar 2018 14:37:04	S	Std
5.0 - 1	55	18921	-	5.0000	245.1	PPB	13 Mar 2018 14:39:12	S	Std
7.5 - 1	57.5	27349	-	7.5000	245.1	PPB	13 Mar 2018 14:41:19	S	Std
10.0 - 1	510	37017	-	10.0000	245.1	PPB	13 Mar 2018 14:43:26	S	Std
ICV41 - 1	ICV41	14899	4.0106	-245.1		PPB	13 Mar 2018 14:54:29	U	SMPL
ICB41 - 1	ICB41	-141	-0.0772	-245.1		PPB	13 Mar 2018 14:56:35	U	SMPL
CCV51 - 1	CCV51	19041	5.1364	-245.1		PPB	13 Mar 2018 14:58:43	U	SMPL
CCB51 - 1	CCB51	-120	-0.0714	-245.1		PPB	13 Mar 2018 15:00:49	U	SMPL
CRA - 1	CRA	354	0.0574	-245.1		PPB	13 Mar 2018 15:02:57	U	SMPL
HighStd - 1	HighStd	37228	10.0796	-245.1		PPB	13 Mar 2018 15:05:03	U	SMPL
ChkStd - 1	ChkStd	24903	6.7297	-245.1		PPB	13 Mar 2018 15:07:10	U	SMPL
PB107254BL - 1	PBW	-48	-0.0519	-245.1		PPB	13 Mar 2018 15:12:12	U	SMPL
PB107254BS - 1	LCSW	13437	3.6133	-245.1		PPB	13 Mar 2018 15:14:19	U	SMPL
J1868-01 - 1	030818-TIDO-F-D-B	-267	-0.1114	-245.1		PPB	13 Mar 2018 15:16:27	U	SMPL
J1868-02 - 1	030818-TIDO-F-D-S	-175	-0.0864	-245.1		PPB	13 Mar 2018 15:18:35	U	SMPL
J1868-03 - 1	030818-TIDO-F-U-B	-148	-0.0791	-245.1		PPB	13 Mar 2018 15:20:43	U	SMPL
J1868-04 - 1	030818-TIDO-F-U-S	-136	-0.0758	-245.1		PPB	13 Mar 2018 15:22:53	U	SMPL
J1869-01 - 1	030618-JETT-E-D-B	-127	-0.0734	-245.1		PPB	13 Mar 2018 15:25:00	U	SMPL
CCV52 - 1	CCV52	18535	4.9989	-245.1		PPB	13 Mar 2018 15:27:06	U	SMPL
CCB52 - 1	CCB52	-129	-0.0739	-245.1		PPB	13 Mar 2018 15:29:13	U	SMPL
J1869-02 - 1	030618-JETT-E-D-S	-157	-0.0815	-245.1		PPB	13 Mar 2018 15:31:20	U	SMPL
J1869-03 - 1	030618-JETT-E-U-B	-135	-0.0755	-245.1		PPB	13 Mar 2018 15:33:26	U	SMPL
J1869-04 - 1	030618-JETT-E-U-S	-147	-0.0788	-245.1		PPB	13 Mar 2018 15:35:33	U	SMPL
J1875-01 - 1	15220032-1	-20	-0.0443	-245.1		PPB	13 Mar 2018 15:37:40	U	SMPL
J1875-01DUP - 1	15220032-1DUP	69	-0.0201	-245.1		PPB	13 Mar 2018 15:39:48	U	SMPL
J1875-01MS - 1	15220032-1MS	13525	3.6372	-245.1		PPB	13 Mar 2018 15:46:30	U	SMPL
J1875-01MSD - 1	15220032-1MSD	13481	3.6252	-245.1		PPB	13 Mar 2018 15:48:38	U	SMPL
J1875-01LX5 - 1		-185	-0.0891	-245.1		PPB	13 Mar 2018 15:50:47	U	SMPL
J1875-01A - 1		13146	3.5342	-245.1		PPB	13 Mar 2018 15:52:56	U	SMPL
CCV53 - 1	CCV53	18805	5.0723	-245.1		PPB	13 Mar 2018 15:55:03	U	SMPL
CCB53 - 1	CCB53	-135	-0.0755	-245.1		PPB	13 Mar 2018 15:57:11	U	SMPL