

21393928

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

3/15/2018 12:19

Test: Phenolics-mg/d

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	0.966	0.0	0.113	
ICB1	0.001	0.0	0.010	
CCV1	1.037	0.0	0.120	
CCB1	0.004	0.0	0.011	
PB107361BL	0.002	0.0	0.010	
PB107361BS	0.978	0.0	0.114	
J1900-27	2.487	0.0	0.274	Test limit high
J1900-27DLX2	1.239	0.0	0.142	
CCV2	1.027	0.0	0.119	
CCB2	0.003	0.0	0.010	

N 10
Mean 0.774
SD 0.7987
CV% 103.15

AS

Aquakem v. 7.2AQ1

Results from time period:

Thu Mar 15 12:05:23 2018

Thu Mar 15 12:19:18 2018

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.05PPM	A	Phenolics-	P	0.0522	mg/l	3/15/2018 10:11:44	
0.1PPM	A	Phenolics-	P	0.1012	mg/l	3/15/2018 10:11:45	
0.25PPM	A	Phenolics-	P	0.2497	mg/l	3/15/2018 10:11:46	
0.50PPM	A	Phenolics-	P	0.499	mg/l	3/15/2018 10:11:47	
1.0PPM	A	Phenolics-	P	0.9955	mg/l	3/15/2018 10:11:48	
2.0PPM	A	Phenolics-	P	2.0024	mg/l	3/15/2018 10:11:49	
ICV1	S	Phenolics-	P	0.9655	mg/l	3/15/2018 12:05:23	
ICB1	S	Phenolics-	P	0.0011	mg/l	3/15/2018 12:05:24	
CCV1	S	Phenolics-	P	1.0365	mg/l	3/15/2018 12:05:25	
CCB1	S	Phenolics-	P	0.0042	mg/l	3/15/2018 12:05:26	
PB107361BL	S	Phenolics-	P	0.0023	mg/l	3/15/2018 12:05:27	
PB107361BS	S	Phenolics-	P	0.9779	mg/l	3/15/2018 12:05:28	
J1900-27	S	Phenolics-	P	2.4866	mg/l	3/15/2018 12:05:29	
J1900-27DLX2	S	Phenolics-	P	1.2395	mg/l	3/15/2018 12:05:30	
CCV2	S	Phenolics-	P	1.0274	mg/l	3/15/2018 12:19:17	
CCB2	S	Phenolics-	P	0.0027	mg/l	3/15/2018 12:19:18	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

3/15/2018 10:12


Test Phenolics-

Accepted 3/15/2018 10:12

Factor 9.423
Bias 0.010

Coeff. of det. 0.999988

Errors

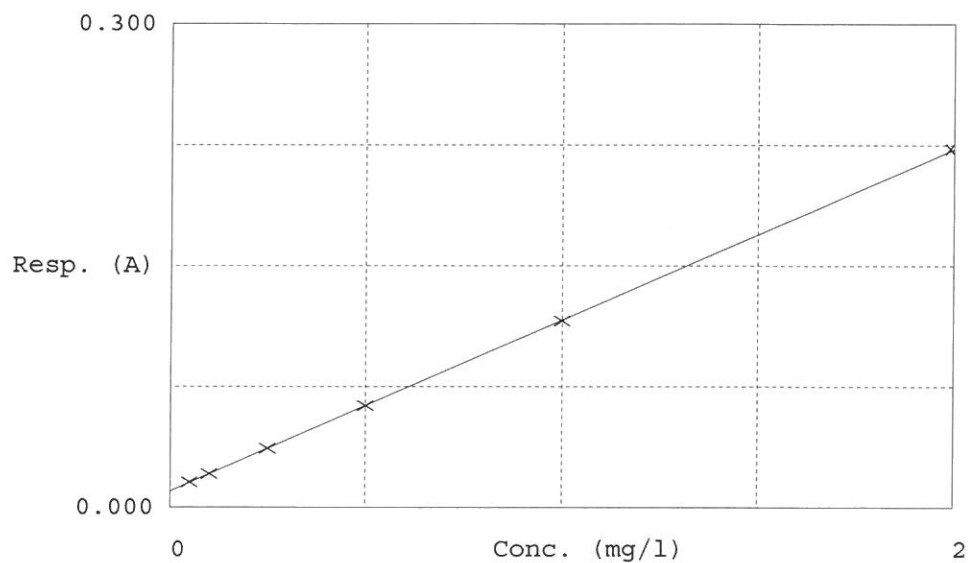

	Calibrator	Response	Calc. con.	Conc.	Errors
1	Phenol-2	0.016	0.0522	0.0500	
2	Phenol-2	0.021	0.1012	0.1000	
3	Phenol-2	0.037	0.2497	0.2500	
4	Phenol-2	0.063	0.4990	0.5000	
5	Phenol-2	0.116	0.9955	1.0000	
6	Phenol-2	0.223	2.0024	2.0000	