

LB94229


7470A

INSTRUMENT ID: CX2

Linear

 μ Abs.:

36079

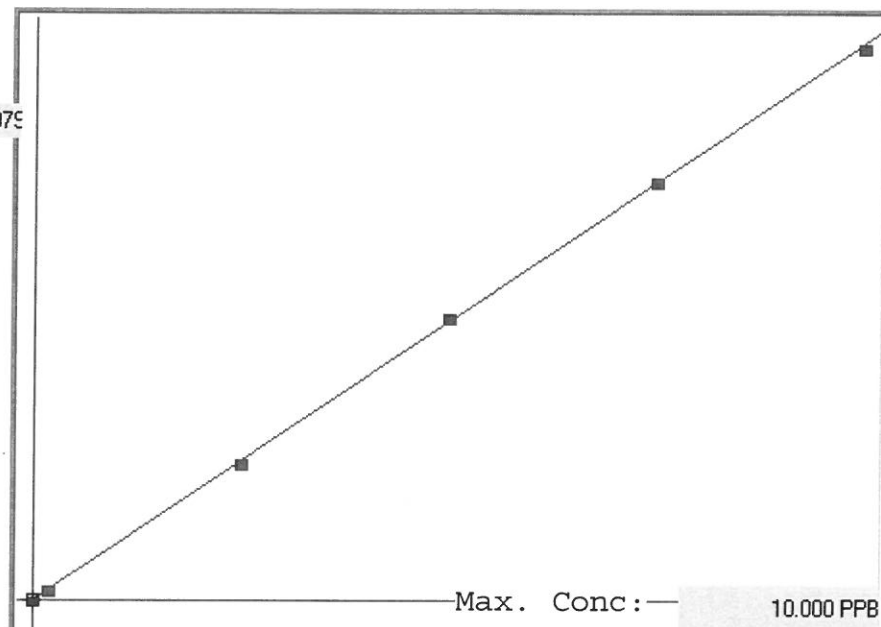

A= 0.0000e+000

B= 2.7592e-004

C= -2.4028e-003

Rho= 0.9999290

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.003	-0.003	-3	0.000	-3				
0.2	0.200	0.190	-0.010	696	0.0 %	696				
2.5	2.500	2.457	-0.043	8913	0.0 %	8913				
5.0	5.000	5.083	0.083	18432	0.0 %	18432				
7.5	7.500	7.521	0.021	27265	0.0 %	27265				
10.0	10.000	9.953	-0.047	36079	0.0 %	36079				

LB94229 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 29 Mar 2018 11:42:02

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-3	-	0.0007	7470A	PPB	29 Mar 2018 11:54:39	S	Std
0.2 - 1	50.2	696	-	0.20007	7470A	PPB	29 Mar 2018 11:56:47	S	Std
2.5 - 1	52.5	8913	-	2.50007	7470A	PPB	29 Mar 2018 11:58:56	S	Std
5.0 - 1	55	18432	-	5.00007	7470A	PPB	29 Mar 2018 12:01:04	S	Std
7.5 - 1	57.5	27265	-	7.50007	7470A	PPB	29 Mar 2018 12:05:43	S	Std
10.0 - 1	59	36079	-	10.00007	7470A	PPB	29 Mar 2018 12:10:16	S	Std
ICV66 - 1	ICV66	13924	3.8396	-7470A	PPB	29 Mar 2018 12:15:30	U	SMPL	
ICB66 - 1	ICB66	-121	-0.0358	-7470A	PPB	29 Mar 2018 12:17:36	U	SMPL	
CCV91 - 1	CCV91	19655	5.4209	-7470A	PPB	29 Mar 2018 12:19:43	U	SMPL	
CCB91 - 1	CCB91	-162	-0.0471	-7470A	PPB	29 Mar 2018 12:21:50	U	SMPL	
CRA - 1	CRA	673	0.1833	-7470A	PPB	29 Mar 2018 12:23:57	U	SMPL	
HighStd - 1	HighStd	35800	9.8756	-7470A	PPB	29 Mar 2018 12:26:04	U	SMPL	
ChkStd - 1	ChkStd	24917	6.8728	-7470A	PPB	29 Mar 2018 12:28:11	U	SMPL	
PB107767BL - 1	PBW	104	0.0263	-7470A	PPB	29 Mar 2018 12:30:20	U	SMPL	
PB107767BS - 1	LCSW	13777	3.7990	-7470A	PPB	29 Mar 2018 12:32:29	U	SMPL	
PB107767TB - 1	PB107720TB	-3	-0.0032	-7470A	PPB	29 Mar 2018 12:37:21	U	SMPL	
J1754-12 - 1	CL-02-032718-A	321	0.0862	-7470A	PPB	29 Mar 2018 12:39:29	U	SMPL	
J1754-12DUP - 1	CL-02-032718-ADUP	286	0.0765	-7470A	PPB	29 Mar 2018 12:41:37	U	SMPL	
J1754-12MS - 1	CL-02-032718-AMS	13555	3.7377	-7470A	PPB	29 Mar 2018 12:43:45	U	SMPL	
J1754-12MSD - 1	CL-02-032718-AMSD	14114	3.8920	-7470A	PPB	29 Mar 2018 12:45:52	U	SMPL	
CCV92 - 1	CCV92	18873	5.2051	-7470A	PPB	29 Mar 2018 12:48:00	U	SMPL	
CCB92 - 1	CCB92	-112	-0.0333	-7470A	PPB	29 Mar 2018 12:50:07	U	SMPL	
J1754-14 - 1	CL-02-032718-B	361	0.0972	-7470A	PPB	29 Mar 2018 12:52:15	U	SMPL	
J1754-16 - 1	CL-02-032718-C	296	0.0793	-7470A	PPB	29 Mar 2018 12:54:22	U	SMPL	
J1754-18 - 1	CL-02-032718-D	413	0.1116	-7470A	PPB	29 Mar 2018 12:56:29	U	SMPL	
J1754-20 - 1	CL-02-032718-E	322	0.0864	-7470A	PPB	29 Mar 2018 12:58:36	U	SMPL	
J1756-12 - 1	OR-01-032718-A	230	0.0611	-7470A	PPB	29 Mar 2018 13:00:43	U	SMPL	
J1756-14 - 1	OR-01-032718-B	357	0.0961	-7470A	PPB	29 Mar 2018 13:02:51	U	SMPL	
J2085-03 - 1	WO-RO-1499	319	0.0856	-7470A	PPB	29 Mar 2018 13:04:59	U	SMPL	
J2086-03 - 1	RS-124023-124035	340	0.0914	-7470A	PPB	29 Mar 2018 13:07:07	U	SMPL	
J2087-03 - 1	JRS-RB201719RT-CV-2530	355	0.0955	-7470A	PPB	29 Mar 2018 13:09:16	U	SMPL	
J2088-02 - 1	TP-2	342	0.0920	-7470A	PPB	29 Mar 2018 13:11:23	U	SMPL	
CCV93 - 1	CCV93	18830	5.1932	-7470A	PPB	29 Mar 2018 13:13:30	U	SMPL	
CCB93 - 1	CCB93	-87	-0.0264	-7470A	PPB	29 Mar 2018 13:15:37	U	SMPL	
J2088-05 - 1	TP-1	339	0.0911	-7470A	PPB	29 Mar 2018 13:17:45	U	SMPL	
J2096-03 - 1	CS-T2	209	0.0553	-7470A	PPB	29 Mar 2018 13:19:52	U	SMPL	
J2100-03 - 1	TP-8-DB	215	0.0569	-7470A	PPB	29 Mar 2018 13:21:59	U	SMPL	
J2100-06 - 1	TP-5-DB	350	0.0942	-7470A	PPB	29 Mar 2018 13:24:06	U	SMPL	
J2102-01 - 1	6978	284	0.0760	-7470A	PPB	29 Mar 2018 13:26:13	U	SMPL	
J2102-02 - 1	6979	334	0.0898	-7470A	PPB	29 Mar 2018 13:28:21	U	SMPL	
J2102-03 - 1	7005	421	0.1138	-7470A	PPB	29 Mar 2018 13:30:29	U	SMPL	
J2102-04 - 1	CHRT25382	57	0.0133	-7470A	PPB	29 Mar 2018 13:32:37	U	SMPL	
PB107768BL - 1	PBW	194	0.0511	-7470A	PPB	29 Mar 2018 13:34:46	U	SMPL	
PB107768BS - 1	LCSW	14101	3.8884	-7470A	PPB	29 Mar 2018 13:36:53	U	SMPL	
CCV94 - 1	CCV94	18731	5.1659	-7470A	PPB	29 Mar 2018 13:39:00	U	SMPL	
CCB94 - 1	CCB94	-105	-0.0314	-7470A	PPB	29 Mar 2018 13:41:08	U	SMPL	
PB107768TB - 1	PB107722TB	206	0.0544	-7470A	PPB	29 Mar 2018 13:46:20	U	SMPL	
J2094-01 - 1	22193-4-5	202	0.0533	-7470A	PPB	29 Mar 2018 13:53:00	U	SMPL	
J2094-01DUP - 1	22193-4-5DUP	198	0.0522	-7470A	PPB	29 Mar 2018 13:55:07	U	SMPL	
J2094-01MS - 1	22193-4-5MS	13810	3.8081	-7470A	PPB	29 Mar 2018 13:57:14	U	SMPL	
J2094-01MSD - 1	22193-4-5MSD	13770	3.7971	-7470A	PPB	29 Mar 2018 13:59:21	U	SMPL	
J2094-05 - 1	22052-53	-80	-0.0245	-7470A	PPB	29 Mar 2018 14:01:29	U	SMPL	
J1754-12LX5 - 1		218	0.0577	-7470A	PPB	29 Mar 2018 14:03:38	U	SMPL	
J1754-12A - 1		13958	3.8489	-7470A	PPB	29 Mar 2018 14:05:46	U	SMPL	
J2094-01LX5 - 1		86	0.0213	-7470A	PPB	29 Mar 2018 14:07:54	U	SMPL	
J2094-01A - 1		14018	3.8655	-7470A	PPB	29 Mar 2018 14:10:02	U	SMPL	
CCV95 - 1	CCV95	18960	5.2291	-7470A	PPB	29 Mar 2018 14:12:09	U	SMPL	
CCB95 - 1	CCB95	-113	-0.0336	-7470A	PPB	29 Mar 2018 14:14:17	U	SMPL	