


7470A

LB94373
INSTRUMENT ID: CV2

Linear

 μ Abs.:

34624

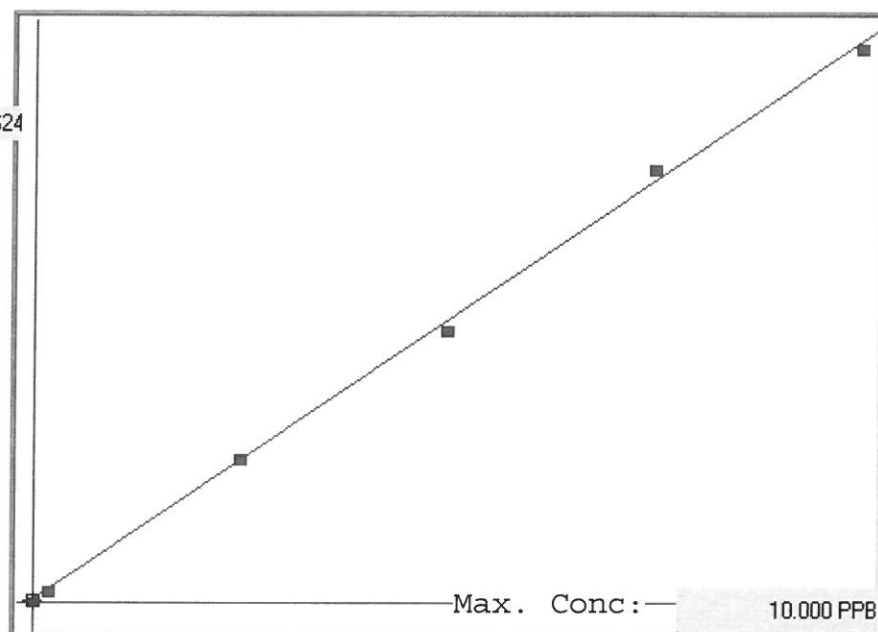

A= 0.0000e+000

B= 2.8659e-004

C= -4.5964e-002

Rho= 0.9994452

Accept= Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.011	-0.011	121	0.000	121				
0.2	0.200	0.192	-0.008	831	0.0 %	831				
2.5	2.500	2.556	0.056	9078	0.0 %	9078				
5.0	5.000	4.858	-0.142	17113	0.0 %	17113				
7.5	7.500	7.728	0.228	27127	0.0 %	27127				
10.0	10.000	9.877	-0.123	34624	0.0 %	34624				

LB94373 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 04 Apr 2018 14:39:23

Sample ID	Extended ID	µ Abs.	Conc.	Std Cond	Method	Units	Date	Type	Type
0.0 - 1	50	121	-	0.0000	7470A	PPB	04 Apr 2018 14:59:32	S	Std
0.2 - 1	50.2	831	-	0.2000	7470A	PPB	04 Apr 2018 15:01:41	S	Std
2.5 - 1	52.5	9078	-	2.5000	7470A	PPB	04 Apr 2018 15:03:49	S	Std
5.0 - 1	55	17113	-	5.0000	7470A	PPB	04 Apr 2018 15:05:58	S	Std
7.5 - 1	57.5	27127	-	7.5000	7470A	PPB	04 Apr 2018 15:08:05	S	Std
10.0 - 1	57.5	34624	-	10.0000	7470A	PPB	04 Apr 2018 15:10:14	S	Std
ICV75 - 1	ICV75	13751	3.8949	-	7470A	PPB	04 Apr 2018 15:15:35	U	SMPL
ICB75 - 1	ICB75	76	-0.0242	-	7470A	PPB	04 Apr 2018 15:17:43	U	SMPL
CCV48 - 1	CCV48	17267	4.9025	-	7470A	PPB	04 Apr 2018 15:19:50	U	SMPL
CCB48 - 1	CCB48	67	-0.0268	-	7470A	PPB	04 Apr 2018 15:21:56	U	SMPL
CRA - 1	CRA	846	0.1965	-	7470A	PPB	04 Apr 2018 15:24:04	U	SMPL
HighStd - 1	HighStd	34609	9.8725	-	7470A	PPB	04 Apr 2018 15:26:10	U	SMPL
ChkStd - 1	ChkStd	24677	7.0261	-	7470A	PPB	04 Apr 2018 15:28:18	U	SMPL
PB107964BL - 1	PBW	213	0.0151	-	7470A	PPB	04 Apr 2018 15:30:26	U	SMPL
PB107964BS - 1	LCSW	12852	3.6372	-	7470A	PPB	04 Apr 2018 15:32:35	U	SMPL
PB107964TB - 1	PB107921TB	150	-0.0030	-	7470A	PPB	04 Apr 2018 15:34:43	U	SMPL
J2185-08 - 1	LOWER-CONCRETE-SLAB-1	249	0.0254	-	7470A	PPB	04 Apr 2018 15:36:52	U	SMPL
J2185-08DUP - 1	LOWER-CONCRETE-SLAB-1DUP	135	-0.0073	-	7470A	PPB	04 Apr 2018 15:39:00	U	SMPL
J2185-08MS - 1	LOWER-CONCRETE-SLAB-1MS	13294	3.7639	-	7470A	PPB	04 Apr 2018 15:41:08	U	SMPL
J2185-08MSD - 1	LOWER-CONCRETE-SLAB-1MSD	13694	3.8785	-	7470A	PPB	04 Apr 2018 15:43:15	U	SMPL
CCV49 - 1	CCV49	17462	4.9584	-	7470A	PPB	04 Apr 2018 15:45:22	U	SMPL
CCB49 - 1	CCB49	53	-0.0308	-	7470A	PPB	04 Apr 2018 15:47:30	U	SMPL
J2185-17 - 1	LOWER-CONCRETE-SLAB-2	388	0.0652	-	7470A	PPB	04 Apr 2018 15:49:37	U	SMPL
J2185-08LX5 - 1		262	0.0291	-	7470A	PPB	04 Apr 2018 15:51:44	U	SMPL
J2185-08A - 1		13850	3.9233	-	7470A	PPB	04 Apr 2018 15:53:50	U	SMPL
CCV50 - 1	CCV50	17133	4.8641	-	7470A	PPB	04 Apr 2018 15:55:57	U	SMPL
CCB50 - 1	CCB50	61	-0.0285	-	7470A	PPB	04 Apr 2018 15:58:05	U	SMPL