


7471B

LB94648
INSTRUMENT ID: CV4

Linear

 μ Abs.:

41407

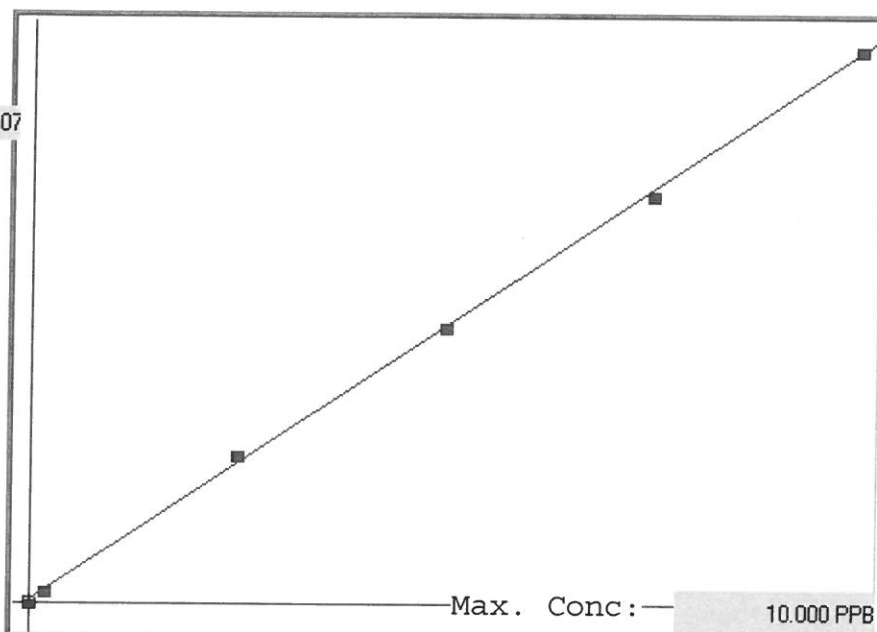

A= 0.0000e+000

B= 2.4351e-004

C= -5.1246e-002

Rho= 0.9997740

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.046	-0.046	23	0.000	23				
0.2	0.200	0.160	-0.040	866	0.0 %	866				
2.5	2.500	2.653	0.153	11105	0.0 %	11105				
5.0	5.000	4.995	-0.005	20725	0.0 %	20725				
7.5	7.500	7.406	-0.094	30625	0.0 %	30625				
10	10.000	10.032	0.032	41407	0.0 %	41407				

LB94648 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 16 Apr 2018 15:27:42

Sample ID	Extended ID	µ Abs	Conc	Std ConcMethod	Units	Date	Type	Type
0.0 - 1	50	23	-	0.00007471B	PPB	16 Apr 2018 15:30:38	S	Std
0.2 - 1	50.2	866	-	0.20007471B	PPB	16 Apr 2018 15:32:55	S	Std
2.5 - 1	52.3	11105	-	2.50007471B	PPB	16 Apr 2018 15:35:13	S	Std
5.0 - 1	55	20725	-	5.00007471B	PPB	16 Apr 2018 15:37:30	S	Std
7.5 - 1	57.7	30625	-	7.50007471B	PPB	16 Apr 2018 15:42:23	S	Std
10 - 1	510	41407	-	10.00007471B	PPB	16 Apr 2018 15:44:40	S	Std
ICV96 - 1	ICV96	16585	3.9873	-7471B	PPB	16 Apr 2018 15:47:46	U	SMPL
ICB96 - 1	ICB96	-189	-0.0973	-7471B	PPB	16 Apr 2018 15:50:02	U	SMPL
CCV44 - 1	CCV44	20844	5.0244	-7471B	PPB	16 Apr 2018 15:52:18	U	SMPL
CCB44 - 1	CCB44	-160	-0.0902	-7471B	PPB	16 Apr 2018 15:54:34	U	SMPL
CRA - 1	CRA	943	0.1784	-7471B	PPB	16 Apr 2018 15:56:50	U	SMPL
HighStd - 1	HighStd	41734	10.1112	-7471B	PPB	16 Apr 2018 15:59:06	U	SMPL
ChkStd - 1	ChkStd	29169	7.0516	-7471B	PPB	16 Apr 2018 16:01:22	U	SMPL
PB108245BL - 1	PBS	-13	-0.0544	-7471B	PPB	16 Apr 2018 16:06:14	U	SMPL
PB108245BS - 1	LCSS	16224	3.8994	-7471B	PPB	16 Apr 2018 16:08:30	U	SMPL
J2354-02 - 1	WC-1-4PT-COMP	4101	0.9474	-7471B	PPB	16 Apr 2018 16:10:47	U	SMPL
J2354-04 - 1	WC-2-4PT-COMP	4209	0.9737	-7471B	PPB	16 Apr 2018 16:13:04	U	SMPL
J2369-01 - 1	RO-1-4	4512	1.0475	-7471B	PPB	16 Apr 2018 16:15:21	U	SMPL
J2369-01DUP - 1	RO-1-4DUP	4685	1.0896	-7471B	PPB	16 Apr 2018 16:17:39	U	SMPL
J2369-01MS - 1	RO-1-4MS	21036	5.0711	-7471B	PPB	16 Apr 2018 16:19:55	U	SMPL
CCV45 - 1	CCV45	20933	5.0461	-7471B	PPB	16 Apr 2018 16:22:11	U	SMPL
CCB45 - 1	CCB45	-142	-0.0858	-7471B	PPB	16 Apr 2018 16:24:28	U	SMPL
J2369-01MSD - 1	RO-1-4MSD	20908	5.0400	-7471B	PPB	16 Apr 2018 16:26:44	U	SMPL
J2370-01 - 1	CG-RO-721194	27	-0.0447	-7471B	PPB	16 Apr 2018 16:28:59	U	SMPL
J2370-03 - 1	CG-RO-7211981	70	-0.0342	-7471B	PPB	16 Apr 2018 16:31:16	U	SMPL
J2370-05 - 1	CG	659619	HIGH	-7471B	PPB	16 Apr 2018 16:33:32	X	
J2386-08 - 1	PAINT-CHIPS-1	1247	0.2524	-7471B	PPB	16 Apr 2018 16:35:23	U	SMPL
J2386-10 - 1	PAINT-CHIPS-2	3371	0.7696	-7471B	PPB	16 Apr 2018 16:38:11	U	SMPL
J2387-01 - 1	20180239-COMPOSITE-A	36842	8.9200	-7471B	PPB	16 Apr 2018 16:40:28	U	SMPL
J2387-02 - 1	20180240-COMPOSITE-B	62993	15.2879	-7471B	PPB	16 Apr 2018 16:42:45	U	SMPL
J2387-03 - 1	20180241-COMPOSITE-C	70066	17.0102	-7471B	PPB	16 Apr 2018 16:45:04	U	SMPL
J2387-04 - 1	20180242-COMPOSITE-D	1093	0.2149	-7471B	PPB	16 Apr 2018 16:47:23	U	SMPL
CCV46 - 1	CCV46	20981	5.0577	-7471B	PPB	16 Apr 2018 16:49:42	U	SMPL
CCB46 - 1	CCB46	-149	-0.0875	-7471B	PPB	16 Apr 2018 16:51:58	U	SMPL
J2387-05 - 1	20180243-COMPOSITE-E	44466	10.7765	-7471B	PPB	16 Apr 2018 16:54:15	U	SMPL
J2387-06 - 1	20180247-FIELD-DUPLICATE	50492	12.2438	-7471B	PPB	16 Apr 2018 16:56:32	U	SMPL
J2387-07 - 1	20180244-AMEND-COMP-A	41530	10.0615	-7471B	PPB	16 Apr 2018 16:58:50	U	SMPL
J2387-08 - 1	20180245-AMEND-COMP-B	57289	13.8990	-7471B	PPB	16 Apr 2018 17:01:09	U	SMPL
J2387-09 - 1	20180246-AMEND-COMP-C	54259	13.1611	-7471B	PPB	16 Apr 2018 17:03:28	U	SMPL
J2393-01 - 1	3-4-DENSE-GRADE-AGG-RCA	5298	1.2388	-7471B	PPB	16 Apr 2018 17:05:47	U	SMPL
J2394-01 - 1	1-1-2-DENSE-GRADE-AGG-RCA	13164	3.1543	-7471B	PPB	16 Apr 2018 17:08:07	U	SMPL
J2395-01 - 1	2-1-2-DENSE-GRADE-AGG-RCA	8300	1.9699	-7471B	PPB	16 Apr 2018 17:10:24	U	SMPL
J2369-01LX5 - 1		1082	0.2122	-7471B	PPB	16 Apr 2018 17:15:20	U	SMPL
J2369-01A - 1		21335	5.1440	-7471B	PPB	16 Apr 2018 17:17:36	U	SMPL
CCV47 - 1	CCV47	20919	5.0427	-7471B	PPB	16 Apr 2018 17:19:52	U	SMPL
CCB47 - 1	CCB47	-170	-0.0926	-7471B	PPB	16 Apr 2018 17:22:10	U	SMPL
J2370-05DLX10 - 1		118837	28.8863	-7471B	PPB	16 Apr 2018 17:24:26	U	SMPL
J2387-02DLX5 - 1		11384	2.7208	-7471B	PPB	16 Apr 2018 17:26:43	U	SMPL
J2387-03DLX5 - 1		13283	3.1832	-7471B	PPB	16 Apr 2018 17:29:04	U	SMPL
J2387-05DLX2 - 1		21495	5.1829	-7471B	PPB	16 Apr 2018 17:31:21	U	SMPL
J2387-06DLX2 - 1		25009	6.0386	-7471B	PPB	16 Apr 2018 17:33:38	U	SMPL
J2387-07DLX2 - 1		20410	4.9187	-7471B	PPB	16 Apr 2018 17:35:55	U	SMPL
J2387-08DLX2 - 1		28314	6.8434	-7471B	PPB	16 Apr 2018 17:38:14	U	SMPL
J2387-09DLX2 - 1		26745	6.4613	-7471B	PPB	16 Apr 2018 17:40:32	U	SMPL
J2370-05DL2X50 - 1		24481	5.9100	-7471B	PPB	16 Apr 2018 17:42:52	U	SMPL
CCV48 - 1	CCV48	20709	4.9915	-7471B	PPB	16 Apr 2018 17:45:10	U	SMPL
CCB48 - 1	CCB48	-171	-0.0929	-7471B	PPB	16 Apr 2018 17:47:27	U	SMPL