


7470A

LB94869
INSTRUMENT ID: CV2

Linear

 μ Abs.:

35283

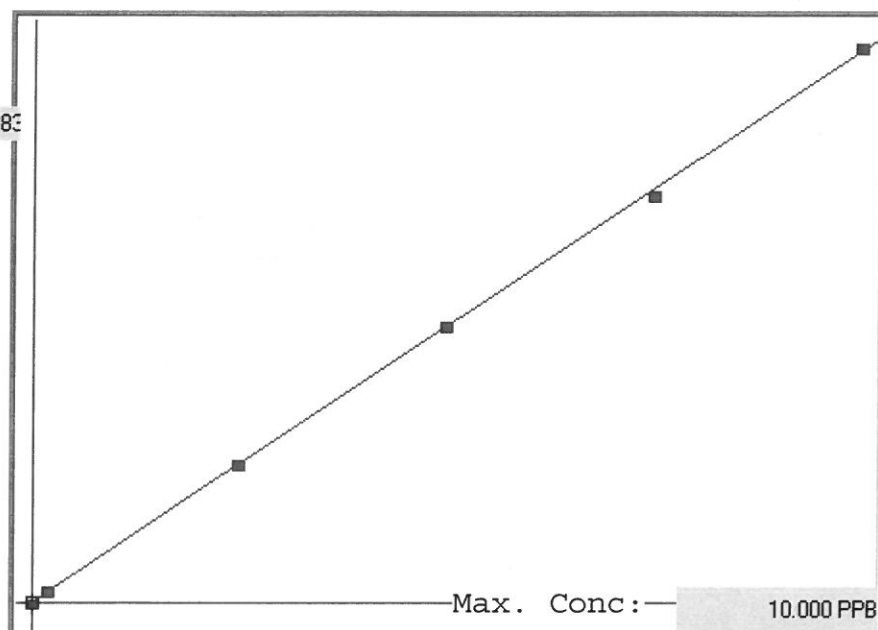

A= 0.0000e+000

B= 2.8557e-004

C= -9.4987e-003

Rho= 0.9998887

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.008	-0.008	5	0.000	5				
0.2	0.200	0.208	0.008	763	0.0 %	763				
2.5	2.500	2.527	0.027	8884	0.0 %	8884				
5.0	5.000	5.018	0.018	17606	0.0 %	17606				
7.5	7.500	7.388	-0.112	25904	0.0 %	25904				
10.0	10.000	10.066	0.066	35283	0.0 %	35283				

LB94869 INSTRUMENT ID : CV1

Method: 7470A		Operator: Admin		Date of Analysis: 25 Apr 2018 10:07:35					
Sample ID	Extended ID	µ Abs.	Conc.	Std. Conc	Method	Units	Date	Type	Type
0.0 - 1	50	5	-	0.0000	7470A	PPB	25 Apr 2018 10:10:06	S	Std
0.2 - 1	50.2	763	-	0.2000	7470A	PPB	25 Apr 2018 10:12:15	S	Std
2.5 - 1	52.5	8884	-	2.5000	7470A	PPB	25 Apr 2018 10:14:23	S	Std
5.0 - 1	55	17606	-	5.0000	7470A	PPB	25 Apr 2018 10:16:31	S	Std
7.5 - 1	57.5	25904	-	7.5000	7470A	PPB	25 Apr 2018 10:18:39	S	Std
10.0 - 1	510	35283	-	10.0000	7470A	PPB	25 Apr 2018 10:23:22	S	Std
ICV13 - 1	ICV13	14216	4.0501	-	7470A	PPB	25 Apr 2018 10:25:50	U	SMPL
ICB13 - 1	ICB13	-163	-0.0560	-	7470A	PPB	25 Apr 2018 10:27:57	U	SMPL
CCV24 - 1	CCV24	18123	5.1658	-	7470A	PPB	25 Apr 2018 10:30:04	U	SMPL
CCB24 - 1	CCB24	-167	-0.0572	-	7470A	PPB	25 Apr 2018 10:32:11	U	SMPL
CRA - 1	CRA	751	0.2050	-	7470A	PPB	25 Apr 2018 10:34:19	U	SMPL
HighStd - 1	HighStd	35273	10.0633	-	7470A	PPB	25 Apr 2018 10:36:25	U	SMPL
ChkStd - 1	ChkStd	24684	7.0394	-	7470A	PPB	25 Apr 2018 10:38:32	U	SMPL
PB108570BL - 1	PBW	-207	-0.0686	-	7470A	PPB	25 Apr 2018 10:40:41	U	SMPL
PB108570BS - 1	LCSW	12714	3.6212	-	7470A	PPB	25 Apr 2018 10:42:51	U	SMPL
PB108570TB - 1	PB108516TB	-96	-0.0369	-	7470A	PPB	25 Apr 2018 10:44:58	U	SMPL
J2151-08 - 1	AU-05-042318-A	-10	-0.0124	-	7470A	PPB	25 Apr 2018 10:47:06	U	SMPL
J2151-08DUP - 1	AU-05-042318-ADUP	14	-0.0055	-	7470A	PPB	25 Apr 2018 10:49:14	U	SMPL
J2151-08MS - 1	AU-05-042318-AMS	13320	3.7943	-	7470A	PPB	25 Apr 2018 10:51:24	U	SMPL
J2151-08MSD - 1	AU-05-042318-AMSD	12398	3.5310	-	7470A	PPB	25 Apr 2018 10:53:30	U	SMPL
CCV25 - 1	CCV25	18063	5.1487	-	7470A	PPB	25 Apr 2018 10:55:37	U	SMPL
CCB25 - 1	CCB25	-146	-0.0512	-	7470A	PPB	25 Apr 2018 10:57:44	U	SMPL
J2151-10 - 1	AU-05-042318-B	22	-0.0032	-	7470A	PPB	25 Apr 2018 10:59:51	U	SMPL
J2151-12 - 1	AU-05-042318-C	95	0.0176	-	7470A	PPB	25 Apr 2018 11:01:58	U	SMPL
J2151-14 - 1	AU-05-042318-D	37	0.0011	-	7470A	PPB	25 Apr 2018 11:04:05	U	SMPL
J2504-03 - 1	KS-RO-238	31	-0.0006	-	7470A	PPB	25 Apr 2018 11:06:11	U	SMPL
J2505-07 - 1	S-3-COMP	30	-0.0009	-	7470A	PPB	25 Apr 2018 11:08:19	U	SMPL
J2506-01 - 1	CB-TCLP-64-0418	65	0.0091	-	7470A	PPB	25 Apr 2018 11:10:26	U	SMPL
J2506-02 - 1	CB-TCLP-VAR-0418	936	0.2578	-	7470A	PPB	25 Apr 2018 11:12:34	U	SMPL
J2508-04 - 1	TP-1	46	0.0036	-	7470A	PPB	25 Apr 2018 11:14:42	U	SMPL
J2508-08 - 1	TP-2	53	0.0056	-	7470A	PPB	25 Apr 2018 11:16:51	U	SMPL
J2508-12 - 1	TP-3	34	0.0002	-	7470A	PPB	25 Apr 2018 11:18:58	U	SMPL
CCV26 - 1	CCV26	17830	5.0822	-	7470A	PPB	25 Apr 2018 11:21:05	U	SMPL
CCB26 - 1	CCB26	-146	-0.0512	-	7470A	PPB	25 Apr 2018 11:23:12	U	SMPL
J2508-16 - 1	TP-4	21	-0.0035	-	7470A	PPB	25 Apr 2018 11:25:19	U	SMPL
J2508-20 - 1	TP-5	19	-0.0041	-	7470A	PPB	25 Apr 2018 11:27:26	U	SMPL
J2508-24 - 1	TP-6	60	0.0076	-	7470A	PPB	25 Apr 2018 11:29:33	U	SMPL
J2509-03 - 1	WS-DRUM	35	0.0005	-	7470A	PPB	25 Apr 2018 11:31:40	U	SMPL
J2512-05 - 1	TP-1-2-WC1	45	0.0034	-	7470A	PPB	25 Apr 2018 11:33:48	U	SMPL
PB108571BL - 1	PBW	26	-0.0021	-	7470A	PPB	25 Apr 2018 11:35:55	U	SMPL
PB108571BS - 1	LCSW	13378	3.8108	-	7470A	PPB	25 Apr 2018 11:38:03	U	SMPL
PB108571TB - 1	PB108523TB	-90	-0.0352	-	7470A	PPB	25 Apr 2018 11:40:12	U	SMPL
J2510-03 - 1	FADW4710L	-2	-0.0101	-	7470A	PPB	25 Apr 2018 11:42:20	U	SMPL
J2510-03DUP - 1	FADW4710LDUP	26	-0.0021	-	7470A	PPB	25 Apr 2018 11:44:27	U	SMPL
CCV27 - 1	CCV27	18047	5.1441	-	7470A	PPB	25 Apr 2018 11:46:34	U	SMPL
CCB27 - 1	CCB27	-150	-0.0523	-	7470A	PPB	25 Apr 2018 11:48:42	U	SMPL
J2510-03MS - 1	FADW4710LMS	13054	3.7183	-	7470A	PPB	25 Apr 2018 11:50:49	U	SMPL
J2510-03MSD - 1	FADW4710LMSD	13126	3.7389	-	7470A	PPB	25 Apr 2018 11:52:57	U	SMPL
PB108572BL - 1	PBW	-106	-0.0398	-	7470A	PPB	25 Apr 2018 11:55:04	U	SMPL
PB108572BS - 1	LCSW	14012	3.9919	-	7470A	PPB	25 Apr 2018 11:57:12	U	SMPL
PB108572TB - 1	PB108522TB	-167	-0.0572	-	7470A	PPB	25 Apr 2018 11:59:20	U	SMPL
J2515-02 - 1	S-1-A	1109	0.3072	-	7470A	PPB	25 Apr 2018 12:01:27	U	SMPL
J2515-04 - 1	S-2-A	1470	0.4103	-	7470A	PPB	25 Apr 2018 12:03:36	U	SMPL
J2515-06 - 1	S-3-A	-65	-0.0281	-	7470A	PPB	25 Apr 2018 12:05:44	U	SMPL
J2515-06DUP - 1	S-3-ADUP	-17	-0.0144	-	7470A	PPB	25 Apr 2018 12:07:52	U	SMPL
J2515-06MS - 1	S-3-AMS	13504	3.8468	-	7470A	PPB	25 Apr 2018 12:10:00	U	SMPL
CV28 - 1	CCV28	17794	5.0719	-	7470A	PPB	25 Apr 2018 12:12:07	U	SMPL
CB28 - 1	CCB28	-152	-0.0529	-	7470A	PPB	25 Apr 2018 12:14:15	U	SMPL
J2515-06MSD - 1	S-3-AMSD	13427	3.8248	-	7470A	PPB	25 Apr 2018 12:16:23	U	SMPL
J2151-08LX5 - 1		-132	-0.0472	-	7470A	PPB	25 Apr 2018 12:18:30	U	SMPL
J2151-08A - 1		13872	3.9519	-	7470A	PPB	25 Apr 2018 12:20:38	U	SMPL
J2510-03LX5 - 1		-138	-0.0489	-	7470A	PPB	25 Apr 2018 12:22:45	U	SMPL
J2510-03A - 1		13728	3.9108	-	7470A	PPB	25 Apr 2018 12:24:52	U	SMPL
J2515-06LX5 - 1		-132	-0.0472	-	7470A	PPB	25 Apr 2018 12:27:00	U	SMPL
J2515-06A - 1		13633	3.8836	-	7470A	PPB	25 Apr 2018 12:29:09	U	SMPL
CV29 - 1	CCV29	18097	5.1584	-	7470A	PPB	25 Apr 2018 12:31:17	U	SMPL
CB29 - 1	CCB29	-166	-0.0569	-	7470A	PPB	25 Apr 2018 12:33:26	U	SMPL