


7470A

LB 94942
INSTRUMENT ID: CY2

Linear

 μ Abs.:

36235

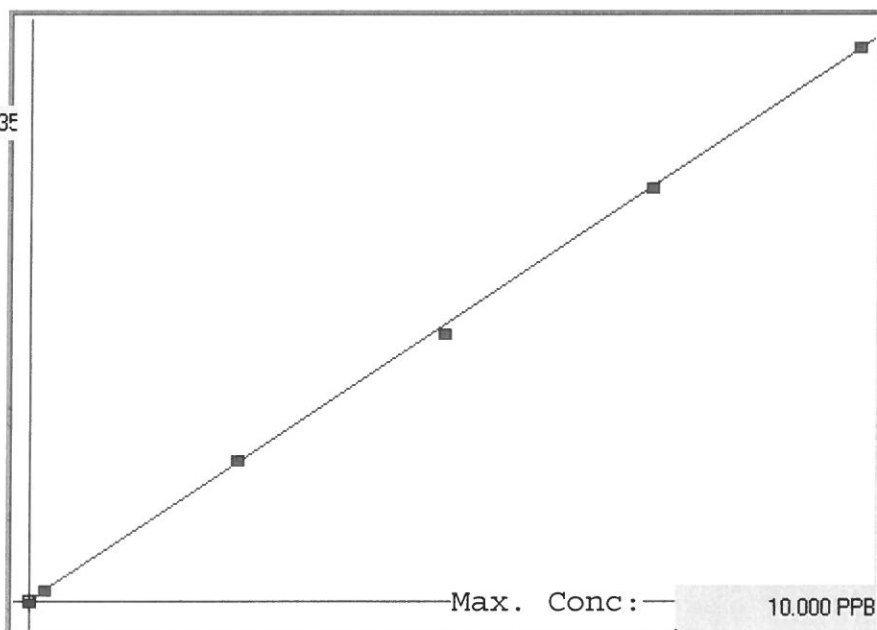

A= 0.0000e+000

B= 2.7704e-004

C= -3.7866e-003

Rho= 0.9998841

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.002	-0.002	5	0.000	5				
0.2	0.200	0.209	0.009	768	0.0 %	768				
2.5	2.500	2.569	0.069	9285	0.0 %	9285				
5.0	5.000	4.886	-0.114	17651	0.0 %	17651				
7.5	7.500	7.504	0.004	27098	0.0 %	27098				
10.0	10.000	10.035	0.035	36235	0.0 %	36235				

LB94942 INSTRUMENT ID : CV1

Method: 7470A		Operator: Admin		Date of Analysis: 27 Apr 2018 10:56:21					
Sample ID	Extended ID	µ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	5	-	0.0000	7470A	PPB	27 Apr 2018 11:06:58	S	Std
0.2 - 1	50.2	768	-	0.2000	7470A	PPB	27 Apr 2018 11:15:26	S	Std
2.5 - 1	52.5	9285	-	2.5000	7470A	PPB	27 Apr 2018 11:17:34	S	Std
5.0 - 1	55	17651	-	5.0000	7470A	PPB	27 Apr 2018 11:19:43	S	Std
7.5 - 1	57.5	27098	-	7.5000	7470A	PPB	27 Apr 2018 11:21:50	S	Std
10.0 - 1	510	36235	-	10.0000	7470A	PPB	27 Apr 2018 11:23:58	S	Std
ICV19 - 1	ICV19	14299	3.9577	-	7470A	PPB	27 Apr 2018 11:26:37	U	SMPL
ICB19 - 1	ICB19	-185	-0.0550	-	7470A	PPB	27 Apr 2018 11:28:44	U	SMPL
CCV52 - 1	CCV52	18154	5.0257	-	7470A	PPB	27 Apr 2018 11:30:51	U	SMPL
CCB52 - 1	CCB52	-182	-0.0542	-	7470A	PPB	27 Apr 2018 11:32:58	U	SMPL
CRA - 1	CRA	708	0.1924	-	7470A	PPB	27 Apr 2018 11:35:06	U	SMPL
HighStd - 1	HighStd	36182	10.0203	-	7470A	PPB	27 Apr 2018 11:37:12	U	SMPL
ChkStd - 1	ChkStd	26125	7.2340	-	7470A	PPB	27 Apr 2018 11:39:19	U	SMPL
PB108642BL - 1	PBW	-258	-0.0753	-	7470A	PPB	27 Apr 2018 11:41:28	U	SMPL
PB108642BS - 1	LCSW	13663	3.7815	-	7470A	PPB	27 Apr 2018 11:43:37	U	SMPL
PB108642TB - 1	PB108612TB	-150	-0.0453	-	7470A	PPB	27 Apr 2018 11:45:45	U	SMPL
J2154-02 - 1	JC-01-042518	-49	-0.0174	-	7470A	PPB	27 Apr 2018 11:47:53	U	SMPL
J2156-06 - 1	HD-05-042518-A	-43	-0.0157	-	7470A	PPB	27 Apr 2018 11:50:01	U	SMPL
J2156-08 - 1	HD-05-042518-B	-28	-0.0115	-	7470A	PPB	27 Apr 2018 11:52:10	U	SMPL
J2156-10 - 1	HD-05-042518-C	-10	-0.0066	-	7470A	PPB	27 Apr 2018 11:54:17	U	SMPL
CCV53 - 1	CCV53	17933	4.9645	-	7470A	PPB	27 Apr 2018 11:56:24	U	SMPL
CCB53 - 1	CCB53	-159	-0.0478	-	7470A	PPB	27 Apr 2018 11:58:30	U	SMPL
J2161-08 - 1	OR-01-042518-A	-39	-0.0146	-	7470A	PPB	27 Apr 2018 12:00:38	U	SMPL
J2161-10 - 1	OR-01-042518-B	-9	-0.0063	-	7470A	PPB	27 Apr 2018 12:02:44	U	SMPL
J2455-44 - 1	TP-1	-19	-0.0091	-	7470A	PPB	27 Apr 2018 12:04:51	U	SMPL
J2455-44DUP - 1	TP-1DUP	-11	-0.0068	-	7470A	PPB	27 Apr 2018 12:06:58	U	SMPL
J2455-44MS - 1	TP-1MS	13824	3.8261	-	7470A	PPB	27 Apr 2018 12:09:05	U	SMPL
J2455-44MSD - 1	TP-1MSD	13353	3.6956	-	7470A	PPB	27 Apr 2018 12:11:13	U	SMPL
J2455-45 - 1	TP-2	-159	-0.0478	-	7470A	PPB	27 Apr 2018 12:13:21	U	SMPL
J2455-46 - 1	TP-3	-50	-0.0176	-	7470A	PPB	27 Apr 2018 12:15:29	U	SMPL
J2455-47 - 1	TP-4	-20	-0.0093	-	7470A	PPB	27 Apr 2018 12:17:38	U	SMPL
J2549-04 - 1	SP-A	-29	-0.0118	-	7470A	PPB	27 Apr 2018 12:19:45	U	SMPL
CCV54 - 1	CCV54	18114	5.0146	-	7470A	PPB	27 Apr 2018 12:21:52	U	SMPL
CCB54 - 1	CCB54	-177	-0.0528	-	7470A	PPB	27 Apr 2018 12:23:59	U	SMPL
J2549-08 - 1	SP-B	-41	-0.0151	-	7470A	PPB	27 Apr 2018 12:26:07	U	SMPL
J2549-12 - 1	SP-C	-26	-0.0110	-	7470A	PPB	27 Apr 2018 12:28:14	U	SMPL
J2549-16 - 1	SP-D	-34	-0.0132	-	7470A	PPB	27 Apr 2018 12:30:21	U	SMPL
J2564-02 - 1	LS-UB-27176	72	0.0162	-	7470A	PPB	27 Apr 2018 12:32:29	U	SMPL
PB108657BL - 1	PBW	-53	-0.0185	-	7470A	PPB	27 Apr 2018 12:34:36	U	SMPL
PB108657BS - 1	LCSW	12988	3.5945	-	7470A	PPB	27 Apr 2018 12:36:44	U	SMPL
J2564-06 - 1	LS-UB-102	129807	35.9586	-	7470A	PPB	27 Apr 2018 12:38:52	U	SMPL
J2564-06DUP - 1	LS-UB-102DUP	129066	35.7533	-	7470A	PPB	27 Apr 2018 12:43:50	U	SMPL
J2564-06MS - 1	LS-UB-102MS	136858	37.9120	-	7470A	PPB	27 Apr 2018 12:48:52	U	SMPL
J2564-06MSD - 1	LS-UB-102MSD	136672	37.8605	-	7470A	PPB	27 Apr 2018 12:55:58	U	SMPL
CCV55 - 1	CCV55	17385	4.8126	-	7470A	PPB	27 Apr 2018 12:58:05	U	SMPL
CCB55 - 1	CCB55	-210	-0.0620	-	7470A	PPB	27 Apr 2018 13:00:37	U	SMPL
J2455-44LX5 - 1		-41	-0.0151	-	7470A	PPB	27 Apr 2018 13:02:46	U	SMPL
J2455-44A - 1		15129	4.1876	-	7470A	PPB	27 Apr 2018 13:04:53	U	SMPL
J2564-06LX5 - 1		27467	7.6058	-	7470A	PPB	27 Apr 2018 13:07:00	U	SMPL
J2564-06A - 1		141323	39.1490	-	7470A	PPB	27 Apr 2018 13:09:07	U	SMPL
J2564-06DLX10 - 1		12689	3.5116	-	7470A	PPB	27 Apr 2018 13:11:16	U	SMPL
J2564-06DUPDLX10 - 1		13274	3.6737	-	7470A	PPB	27 Apr 2018 13:13:47	U	SMPL
J2564-06MSDLX10 - 1		14277	3.9516	-	7470A	PPB	27 Apr 2018 13:15:56	U	SMPL
J2564-06MSDDLX10 - 1		14275	3.9510	-	7470A	PPB	27 Apr 2018 13:18:05	U	SMPL
J2564-06LDLX50 - 1		2583	0.7118	-	7470A	PPB	27 Apr 2018 13:20:14	U	SMPL
J2564-06ADLX10 - 1		14717	4.0735	-	7470A	PPB	27 Apr 2018 13:25:10	U	SMPL
CCV56 - 1	CCV56	18371	5.0858	-	7470A	PPB	27 Apr 2018 13:27:17	U	SMPL
CCB56 - 1	CCB56	-169	-0.0506	-	7470A	PPB	27 Apr 2018 13:29:25	U	SMPL