


7471B

LB95056
INSTRUMENT ID: CV1

Linear

 μ Abs.:

47258

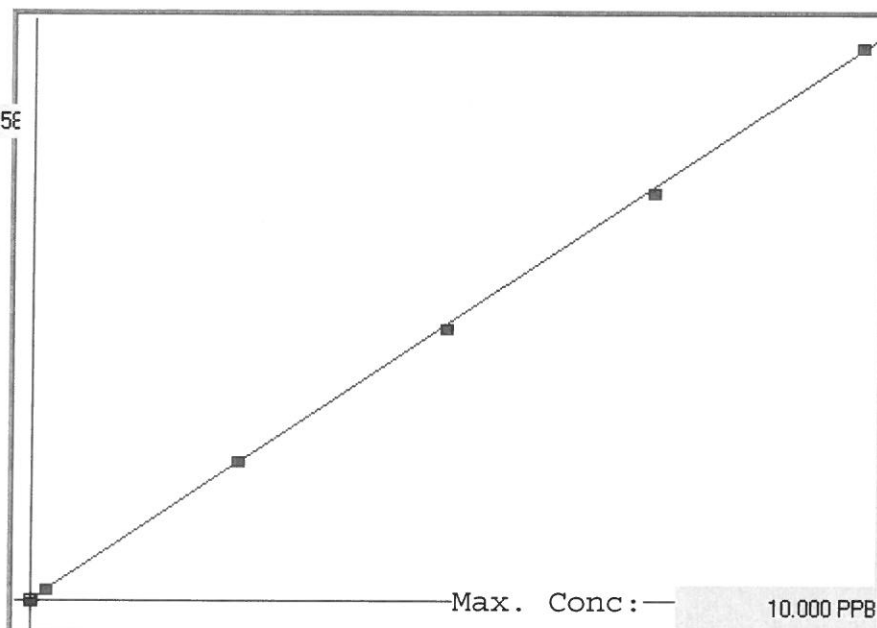

A= 0.0000e+000

B= 2.1312e-004

C= -9.2743e-003

Rho= 0.9999151

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.002	-0.002	34	0.000	34				
0.2	0.200	0.201	0.001	988	0.0 %	988				
2.5	2.500	2.548	0.048	12001	0.0 %	12001				
5.0	5.000	4.973	-0.027	23380	0.0 %	23380				
7.5	7.500	7.417	-0.083	34844	0.0 %	34844				
10.0	10.000	10.062	0.062	47258	0.0 %	47258				

LB95056 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 02 May 2018 17:13:46

Sample ID	Extended ID	µ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	34	-	0.0000	7471B	PPB	02 May 2018 17:15:55	S	Std
0.2 - 1	50.2	988	-	0.2000	7471B	PPB	02 May 2018 17:18:12	S	Std
2.5 - 1	52.5	12001	-	2.5000	7471B	PPB	02 May 2018 17:20:30	S	Std
5.0 - 1	55	23380	-	5.0000	7471B	PPB	02 May 2018 17:22:47	S	Std
7.5 - 1	57.5	34844	-	7.5000	7471B	PPB	02 May 2018 17:25:05	S	Std
10.0 - 1	510	47258	-	10.0000	7471B	PPB	02 May 2018 17:27:22	S	Std
ICV27 - 1	ICV27	17823	3.7891	-	7471B	PPB	02 May 2018 17:30:03	U	SMPL
ICB27 - 1	ICB27	-126	-0.0361	-	7471B	PPB	02 May 2018 17:32:19	U	SMPL
CCV92 - 1	CCV92	21865	4.6506	-	7471B	PPB	02 May 2018 17:34:36	U	SMPL
CCB92 - 1	CCB92	-124	-0.0357	-	7471B	PPB	02 May 2018 17:36:51	U	SMPL
CRA - 1	CRA	980	0.1996	-	7471B	PPB	02 May 2018 17:39:08	U	SMPL
HighStd - 1	HighStd	47451	10.1034	-	7471B	PPB	02 May 2018 17:41:24	U	SMPL
ChkStd - 1	ChkStd	31995	6.8095	-	7471B	PPB	02 May 2018 17:43:40	U	SMPL
PB108796BL - 1	PBS	-212	-0.0545	-	7471B	PPB	02 May 2018 17:45:59	U	SMPL
PB108796BS - 1	LCSS	15934	3.3866	-	7471B	PPB	02 May 2018 17:48:17	U	SMPL
J2652-09 - 1	COMPOSITE-P4-WC	6217	1.3157	-	7471B	PPB	02 May 2018 17:50:34	U	SMPL
J2652-10 - 1	COMPOSITE-P5-WC	11681	2.4802	-	7471B	PPB	02 May 2018 17:52:51	U	SMPL
J2652-11 - 1	AMENDED-COMPOSITE-P4-WC	6189	1.3097	-	7471B	PPB	02 May 2018 17:55:09	U	SMPL
J2652-12 - 1	AMENDED-COMPOSITE-P5-WC	12025	2.5535	-	7471B	PPB	02 May 2018 17:57:27	U	SMPL
J2665-01 - 1	ES-RO-124030	496	0.0964	-	7471B	PPB	02 May 2018 17:59:43	U	SMPL
CCV93 - 1	CCV93	22626	4.8128	-	7471B	PPB	02 May 2018 18:01:59	U	SMPL
CCB93 - 1	CCB93	-199	-0.0517	-	7471B	PPB	02 May 2018 18:04:15	U	SMPL
J2665-05 - 1	ES-RT-2655	2498	0.5231	-	7471B	PPB	02 May 2018 18:06:31	U	SMPL
J2665-09 - 1	ES-RT-1871	2736	0.5738	-	7471B	PPB	02 May 2018 18:08:47	U	SMPL
J2666-01 - 1	CURB-A-CONCRETE	166	0.0261	-	7471B	PPB	02 May 2018 18:11:03	U	SMPL
J2666-03 - 1	CURB-A-PAINT-CHIPS	737	0.1478	-	7471B	PPB	02 May 2018 18:13:19	U	SMPL
J2666-05 - 1	CURB-B-CONCRETE	83	0.0084	-	7471B	PPB	02 May 2018 18:15:35	U	SMPL
J2666-07 - 1	CURB-B-PAINT-CHIPS	120	0.0163	-	7471B	PPB	02 May 2018 18:17:52	U	SMPL
J2667-02 - 1	285-147-7212002-RB26667	7721	1.6362	-	7471B	PPB	02 May 2018 18:20:09	U	SMPL
J2667-05 - 1	155-348-281	13278	2.8205	-	7471B	PPB	02 May 2018 18:22:26	U	SMPL
J2667-08 - 1	137-132-165	6896	1.4604	-	7471B	PPB	02 May 2018 18:24:44	U	SMPL
J2682-01 - 1	EPE-F-6(0-5)	5839	1.2351	-	7471B	PPB	02 May 2018 18:27:00	U	SMPL
CCV94 - 1	CCV94	22238	4.7301	-	7471B	PPB	02 May 2018 18:29:16	U	SMPL
CCB94 - 1	CCB94	-217	-0.0555	-	7471B	PPB	02 May 2018 18:31:32	U	SMPL
J2682-01DUP - 1	EPE-F-6(0-5)DUP	5767	1.2198	-	7471B	PPB	02 May 2018 18:38:38	U	SMPL
J2682-01MS - 1	EPE-F-6(0-5)MS	23458	4.9901	-	7471B	PPB	02 May 2018 18:40:54	U	SMPL
J2682-01MSD - 1	EPE-F-6(0-5)MSD	23258	4.9474	-	7471B	PPB	02 May 2018 18:43:10	U	SMPL
J2682-01LX5 - 1		1068	0.2183	-	7471B	PPB	02 May 2018 18:45:27	U	SMPL
J2682-01A - 1		23324	4.9615	-	7471B	PPB	02 May 2018 18:47:45	U	SMPL
CCV95 - 1	CCV95	22321	4.7478	-	7471B	PPB	02 May 2018 18:50:02	U	SMPL
CCB95 - 1	CCB95	-233	-0.0589	-	7471B	PPB	02 May 2018 18:52:19	U	SMPL