


7470A

LB95069
INSTRUMENT ID: CV4

Linear

 μ Abs.:

36962

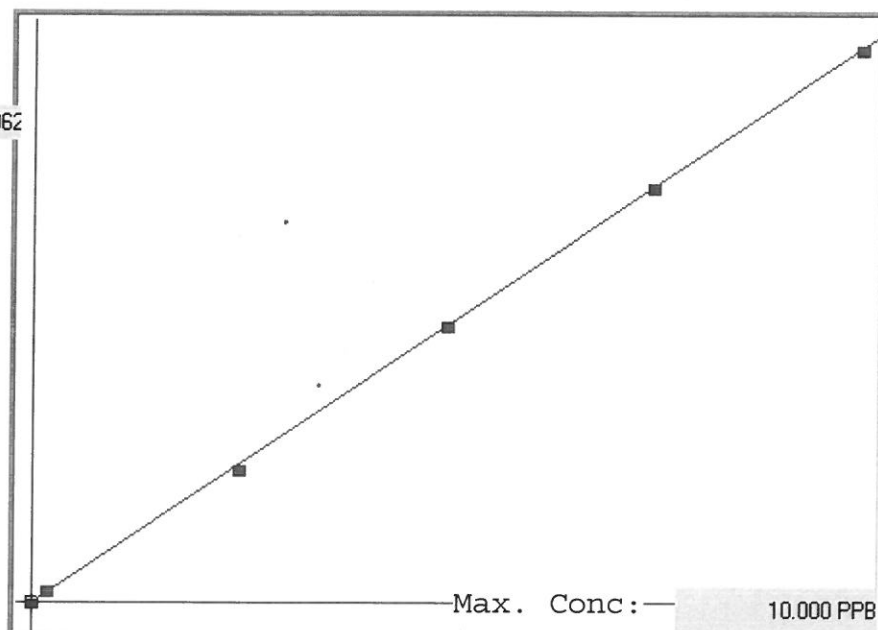

A= 0.0000e+000

B= 2.7010e-004

C= 1.8257e-002

Rho= 0.9999517

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.012	0.012	-22	0.000	-22				
0.2	0.200	0.239	0.039	819	0.0 %	819				
2.5	2.500	2.424	-0.076	8905	0.0 %	8905				
5.0	5.000	5.006	0.006	18465	0.0 %	18465				
7.5	7.500	7.517	0.017	27763	0.0 %	27763				
10.0	10.000	10.002	0.002	36962	0.0 %	36962				

LB95069 INSTRUMENT ID : CV1

Method: 7470A		Operator: Admin		Date of Analysis: 03 May 2018 10:59:35						
Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type	
0.0 - 1	50	-22	-	0.0000	7470A	PPB	03 May 2018 11:03:53	S	Std	
0.2 - 1	50.2	819	-	0.2000	7470A	PPB	03 May 2018 11:06:01	S	Std	
2.5 - 1	52.5	8905	-	2.5000	7470A	PPB	03 May 2018 11:08:10	S	Std	
5.0 - 1	55	18465	-	5.0000	7470A	PPB	03 May 2018 11:10:18	S	Std	
7.5 - 1	57.5	27763	-	7.5000	7470A	PPB	03 May 2018 11:12:26	S	Std	
10.0 - 1	510	36962	-	10.0000	7470A	PPB	03 May 2018 11:14:34	S	Std	
ICV27 - 1	ICV27	13987	3.7962	-	7470A	PPB	03 May 2018 11:17:29	U	SMPL	
ICB27 - 1	ICB27	-184	-0.0314	-	7470A	PPB	03 May 2018 11:19:35	U	SMPL	
CCV01 - 1	CCV01	18576	5.0357	-	7470A	PPB	03 May 2018 11:21:43	U	SMPL	
CCB01 - 1	CCB01	-184	-0.0314	-	7470A	PPB	03 May 2018 11:23:49	U	SMPL	
CRA - 1	CRA	683	0.2027	-	7470A	PPB	03 May 2018 11:25:56	U	SMPL	
HighStd - 1	HighStd	36954	9.9997	-	7470A	PPB	03 May 2018 11:28:03	U	SMPL	
ChkStd - 1	ChkStd	25673	6.9526	-	7470A	PPB	03 May 2018 11:30:10	U	SMPL	
PB108842BL - 1	PBW	-240	-0.0466	-	7470A	PPB	03 May 2018 11:32:19	U	SMPL	
PB108842BS - 1	LCSW	14203	3.8545	-	7470A	PPB	03 May 2018 11:34:27	U	SMPL	
PB108842TB - 1	PB108793TB	-132	-0.0174	-	7470A	PPB	03 May 2018 11:36:35	U	SMPL	
J2652-21 - 1	COMPOSITE-P4-WC	-15	0.0142	-	7470A	PPB	03 May 2018 11:38:43	U	SMPL	
J2652-21DUP - 1	COMPOSITE-P4-WC DUP	3	0.0191	-	7470A	PPB	03 May 2018 11:40:52	U	SMPL	
J2652-21MS - 1	COMPOSITE-P4-WC MS	13983	3.7951	-	7470A	PPB	03 May 2018 11:43:00	U	SMPL	
J2652-21MSD - 1	COMPOSITE-P4-WC MSD	14200	3.8537	-	7470A	PPB	03 May 2018 11:45:07	U	SMPL	
CCV02 - 1	CCV02	18187	4.9306	-	7470A	PPB	03 May 2018 11:47:14	U	SMPL	
CCB02 - 1	CCB02	-200	-0.0358	-	7470A	PPB	03 May 2018 11:49:21	U	SMPL	
J2652-22 - 1	COMPOSITE-P5-WC	-13	0.0147	-	7470A	PPB	03 May 2018 11:51:29	U	SMPL	
J2652-23 - 1	AMENDED-COMPOSITE-P4-WC	-16	0.0139	-	7470A	PPB	03 May 2018 11:53:36	U	SMPL	
J2652-24 - 1	AMENDED-COMPOSITE-P5-WC	-3	0.0174	-	7470A	PPB	03 May 2018 11:55:43	U	SMPL	
J2665-04 - 1	ES-RO-124030	1	0.0185	-	7470A	PPB	03 May 2018 11:57:50	U	SMPL	
J2665-08 - 1	ES-RT-2655	5	0.0196	-	7470A	PPB	03 May 2018 11:59:57	U	SMPL	
J2665-12 - 1	ES-RT-1871	3	0.0191	-	7470A	PPB	03 May 2018 12:02:05	U	SMPL	
J2666-02 - 1	CURB-A-CONCRETE	0	0.0183	-	7470A	PPB	03 May 2018 12:04:13	U	SMPL	
J2666-04 - 1	CURB-A-PAINT-CHIPS	-15	0.0142	-	7470A	PPB	03 May 2018 12:06:21	U	SMPL	
J2666-06 - 1	CURB-B-CONCRETE	9	0.0207	-	7470A	PPB	03 May 2018 12:08:30	U	SMPL	
J2666-08 - 1	CURB-B-PAINT-CHIPS	-6	0.0166	-	7470A	PPB	03 May 2018 12:10:36	U	SMPL	
CCV03 - 1	CCV03	18682	5.0643	-	7470A	PPB	03 May 2018 12:12:43	U	SMPL	
CCB03 - 1	CCB03	-181	-0.0306	-	7470A	PPB	03 May 2018 12:14:50	U	SMPL	
J2667-01 - 1	PUMP-HOUSE	-26	0.0112	-	7470A	PPB	03 May 2018 12:16:58	U	SMPL	
J2667-04 - 1	285-147-7212002-RB26667	-11	0.0153	-	7470A	PPB	03 May 2018 12:19:05	U	SMPL	
J2667-07 - 1	155-348-281	-3	0.0174	-	7470A	PPB	03 May 2018 12:21:12	U	SMPL	
J2667-10 - 1	137-132-165	4	0.0193	-	7470A	PPB	03 May 2018 12:23:19	U	SMPL	
J2669-02 - 1	SU-03-050118-A	-6	0.0166	-	7470A	PPB	03 May 2018 12:25:26	U	SMPL	
J2669-04 - 1	SU-03-050118-B	3	0.0191	-	7470A	PPB	03 May 2018 12:27:34	U	SMPL	
PB108843BL - 1	PBW	-8	0.0161	-	7470A	PPB	03 May 2018 12:29:42	U	SMPL	
PB108843BS - 1	LCSW	14077	3.8205	-	7470A	PPB	03 May 2018 12:31:50	U	SMPL	
PB108843TB - 1	PB108795TB	-115	-0.0128	-	7470A	PPB	03 May 2018 12:33:59	U	SMPL	
J2667-15 - 1	GROUNDWATER	-10	0.0156	-	7470A	PPB	03 May 2018 12:36:06	U	SMPL	
CCV04 - 1	CCV04	18631	5.0506	-	7470A	PPB	03 May 2018 12:38:13	U	SMPL	
CCB04 - 1	CCB04	-196	-0.0347	-	7470A	PPB	03 May 2018 12:40:20	U	SMPL	
J2667-15DUP - 1	GROUNDWATERDUP	-27	0.0110	-	7470A	PPB	03 May 2018 12:42:28	U	SMPL	
J2667-15MS - 1	GROUNDWATERMS	12076	3.2800	-	7470A	PPB	03 May 2018 12:44:36	U	SMPL	
J2667-15MSD - 1	GROUNDWATERMSD	14082	3.8219	-	7470A	PPB	03 May 2018 12:46:43	U	SMPL	
PB108844BL - 1	PBW	-125	-0.0155	-	7470A	PPB	03 May 2018 12:48:50	U	SMPL	
PB108844BS - 1	LCSW	14197	3.8529	-	7470A	PPB	03 May 2018 12:50:58	U	SMPL	
J2667-11 - 1	GROUNDWATER	681	0.2022	-	7470A	PPB	03 May 2018 12:52:40	U	SMPL	
J2667-11DUP - 1	GROUNDWATERDUP	599	0.1800	-	7470A	PPB	03 May 2018 12:54:47	U	SMPL	
J2667-11MS - 1	GROUNDWATERMS	16952	4.5971	-	7470A	PPB	03 May 2018 13:01:55	U	SMPL	
J2667-11MSD - 1	GROUNDWATERMSD	16929	4.5908	-	7470A	PPB	03 May 2018 13:04:04	U	SMPL	
CCV05 - 1	CCV05	18836	5.1059	-	7470A	PPB	03 May 2018 13:06:11	U	SMPL	
CCB05 - 1	CCB05	-157	-0.0241	-	7470A	PPB	03 May 2018 13:08:18	U	SMPL	
J2652-21LX5 - 1		-28	0.0107	-	7470A	PPB	03 May 2018 13:10:26	U	SMPL	
J2652-21A - 1		14161	3.8432	-	7470A	PPB	03 May 2018 13:12:33	U	SMPL	
J2667-15LX5 - 1		-113	-0.0123	-	7470A	PPB	03 May 2018 13:14:40	U	SMPL	
J2667-15A - 1		13664	3.7090	-	7470A	PPB	03 May 2018 13:16:47	U	SMPL	
J2667-11LX5 - 1		307	0.1012	-	7470A	PPB	03 May 2018 13:18:54	U	SMPL	
J2667-11A - 1		16792	4.5538	-	7470A	PPB	03 May 2018 13:21:02	U	SMPL	
CV06 - 1	CCV06	18454	5.0027	-	7470A	PPB	03 May 2018 13:23:09	U	SMPL	
CB06 - 1	CCB06	-149	-0.0220	-	7470A	PPB	03 May 2018 13:25:18	U	SMPL	