


7470A

LB 95188
INSTRUMENT ID: CV4

Linear

 μ Abs.:

37894

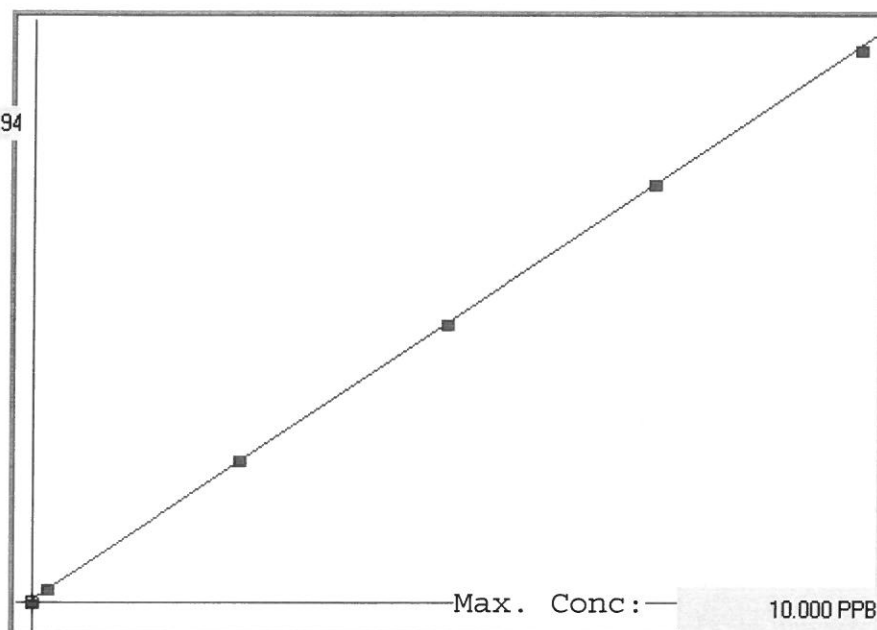

A= 0.0000e+000

B= 2.6383e-004

C= -4.2061e-002

Rho= 0.9999539

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.052	-0.052	-36	0.000	-36				
0.2	0.200	0.213	0.013	968	0.0 %	968				
2.5	2.500	2.532	0.032	9756	0.0 %	9756				
5.0	5.000	5.011	0.011	19151	0.0 %	19151				
7.5	7.500	7.540	0.040	28738	0.0 %	28738				
10.0	10.000	9.956	-0.044	37894	0.0 %	37894				

LB95188 INSTRUMENT ID : CV1

Method: 7470A		Operator: Admin		Date of Analysis: 08 May 2018 12:45:27					
Sample ID	Extended ID	µ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-36	-	0.0000	7470A	PPB	08 May 2018 12:49:16	S	Std
0.2 - 1	50.2	968	-	0.2000	7470A	PPB	08 May 2018 12:51:24	S	Std
2.5 - 1	52.5	9756	-	2.5000	7470A	PPB	08 May 2018 12:53:32	S	Std
5.0 - 1	55	19151	-	5.0000	7470A	PPB	08 May 2018 12:55:40	S	Std
7.5 - 1	57.5	28738	-	7.5000	7470A	PPB	08 May 2018 12:57:48	S	Std
10.0 - 1	510	37894	-	10.0000	7470A	PPB	08 May 2018 12:59:56	S	Std
ICV34 - 1	ICV34	14015	3.6556	-	7470A	PPB	08 May 2018 13:02:38	U	SMPL
ICB34 - 1	ICB34	5	-0.0407	-	7470A	PPB	08 May 2018 13:07:28	U	SMPL
CCV54 - 1	CCV54	18611	4.8682	-	7470A	PPB	08 May 2018 13:09:34	U	SMPL
CCB54 - 1	CCB54	-122	-0.0742	-	7470A	PPB	08 May 2018 13:11:41	U	SMPL
CRA - 1	CRA	932	0.2038	-	7470A	PPB	08 May 2018 13:13:49	U	SMPL
HighStd - 1	HighStd	37977	9.9776	-	7470A	PPB	08 May 2018 13:15:55	U	SMPL
ChkStd - 1	ChkStd	27205	7.1356	-	7470A	PPB	08 May 2018 13:18:02	U	SMPL
PB109011BL - 1	PBW	-215	-0.0988	-	7470A	PPB	08 May 2018 13:20:11	U	SMPL
PB109011BS - 1	LCSW	13643	3.5574	-	7470A	PPB	08 May 2018 13:22:20	U	SMPL
PB109011TB - 1	PB108943TB	-173	-0.0877	-	7470A	PPB	08 May 2018 13:24:28	U	SMPL
J2675-02 - 1	HR-06-050418	-64	-0.0589	-	7470A	PPB	08 May 2018 13:26:36	U	SMPL
J2675-02DUP - 1	HR-06-050418DUP	-14	-0.0458	-	7470A	PPB	08 May 2018 13:28:44	U	SMPL
J2675-02MS - 1	HR-06-050418MS	13607	3.5479	-	7470A	PPB	08 May 2018 13:30:52	U	SMPL
J2675-02MSD - 1	HR-06-050418MSD	13802	3.5994	-	7470A	PPB	08 May 2018 13:32:59	U	SMPL
CCV55 - 1	CCV55	18410	4.8151	-	7470A	PPB	08 May 2018 13:35:06	U	SMPL
CCB55 - 1	CCB55	-117	-0.0729	-	7470A	PPB	08 May 2018 13:37:12	U	SMPL
J2677-02 - 1	OK-03-050418	-68	-0.0600	-	7470A	PPB	08 May 2018 13:39:19	U	SMPL
J2677-04 - 1	OK-01-050718	-64	-0.0589	-	7470A	PPB	08 May 2018 13:41:26	U	SMPL
J2680-02 - 1	PL-02-050418-A	-76	-0.0621	-	7470A	PPB	08 May 2018 13:43:33	U	SMPL
J2680-04 - 1	PL-02-050418-B	-54	-0.0563	-	7470A	PPB	08 May 2018 13:45:40	U	SMPL
J2680-06 - 1	PL-02-050418-C	-69	-0.0603	-	7470A	PPB	08 May 2018 13:47:47	U	SMPL
J2680-08 - 1	PL-02-050418-D	-53	-0.0560	-	7470A	PPB	08 May 2018 13:49:54	U	SMPL
J2680-10 - 1	PL-02-050418-E	-40	-0.0526	-	7470A	PPB	08 May 2018 13:52:03	U	SMPL
J2736-03 - 1	MS-SOIL	-15	-0.0460	-	7470A	PPB	08 May 2018 13:54:11	U	SMPL
J2738-01 - 1	CB-TCLP-VAR1-0518	-31	-0.0502	-	7470A	PPB	08 May 2018 13:56:19	U	SMPL
J2738-02 - 1	CB-TCLP-VAR2-0518	-45	-0.0539	-	7470A	PPB	08 May 2018 13:58:26	U	SMPL
CCV56 - 1	CCV56	19218	5.0283	-	7470A	PPB	08 May 2018 14:00:33	U	SMPL
CCB56 - 1	CCB56	-193	-0.0930	-	7470A	PPB	08 May 2018 14:02:40	U	SMPL
J2738-03 - 1	CB-TCLP-VAR3-0518	-11	-0.0450	-	7470A	PPB	08 May 2018 14:04:48	U	SMPL
J2738-04 - 1	CB-TCLP-VAR4-0518	-19	-0.0471	-	7470A	PPB	08 May 2018 14:06:56	U	SMPL
J2738-05 - 1	CB-TCLP-VAR5-0518	15	-0.0381	-	7470A	PPB	08 May 2018 14:09:03	U	SMPL
J2754-04 - 1	LS-SOIL-PILE-1A	-33	-0.0508	-	7470A	PPB	08 May 2018 14:11:10	U	SMPL
J2754-08 - 1	LS-SOIL-PILE-1B	-12	-0.0452	-	7470A	PPB	08 May 2018 14:13:17	U	SMPL
J2754-12 - 1	LS-SOIL-PILE-2A	-21	-0.0476	-	7470A	PPB	08 May 2018 14:15:25	U	SMPL
J2754-16 - 1	LS-SOIL-PILE-2B	-25	-0.0487	-	7470A	PPB	08 May 2018 14:17:33	U	SMPL
J2769-04 - 1	NORTH-AVE-TP	-40	-0.0526	-	7470A	PPB	08 May 2018 14:19:41	U	SMPL
PB109012BL - 1	PBW	24	-0.0357	-	7470A	PPB	08 May 2018 14:21:50	U	SMPL
PB109012BS - 1	LCSW	13681	3.5675	-	7470A	PPB	08 May 2018 14:23:57	U	SMPL
CCV57 - 1	CCV57	18592	4.8631	-	7470A	PPB	08 May 2018 14:26:04	U	SMPL
CCB57 - 1	CCB57	-156	-0.0832	-	7470A	PPB	08 May 2018 14:28:12	U	SMPL
PB109012TB - 1	PB108945TB	-46	-0.0542	-	7470A	PPB	08 May 2018 14:30:20	U	SMPL
J2776-02 - 1	JCSA-301	-12	-0.0452	-	7470A	PPB	08 May 2018 14:32:27	U	SMPL
J2776-02DUP - 1	JCSA-301DUP	-8	-0.0442	-	7470A	PPB	08 May 2018 14:34:34	U	SMPL
J2776-02MS - 1	JCSA-301MS	13587	3.5427	-	7470A	PPB	08 May 2018 14:36:41	U	SMPL
J2776-02MSD - 1	JCSA-301MSD	13674	3.5656	-	7470A	PPB	08 May 2018 14:38:48	U	SMPL
PB109013BL - 1	PBW	-118	-0.0732	-	7470A	PPB	08 May 2018 14:40:55	U	SMPL
PB109013BS - 1	LCSW	13498	3.5192	-	7470A	PPB	08 May 2018 14:43:04	U	SMPL
PB109013TB - 1	PB108946TB	-150	-0.0816	-	7470A	PPB	08 May 2018 14:45:12	U	SMPL
J2759-02 - 1	TP-2	-49	-0.0550	-	7470A	PPB	08 May 2018 14:47:20	U	SMPL
J2764-02 - 1	WATER-WELL	-5	-0.0434	-	7470A	PPB	08 May 2018 14:49:27	U	SMPL
CV58 - 1	CCV58	18904	4.9455	-	7470A	PPB	08 May 2018 14:51:34	U	SMPL
CB58 - 1	CCB58	-143	-0.0798	-	7470A	PPB	08 May 2018 14:53:41	U	SMPL
J2764-02DUP - 1	WATER-WELLDUP	-25	-0.0487	-	7470A	PPB	08 May 2018 14:55:49	U	SMPL
J2764-02MS - 1	WATER-WELLS	13776	3.5925	-	7470A	PPB	08 May 2018 14:57:56	U	SMPL
J2764-02MSD - 1	WATER-WELLSMSD	13820	3.6041	-	7470A	PPB	08 May 2018 15:00:03	U	SMPL
PB109017BL - 1	PBW	-160	-0.0843	-	7470A	PPB	08 May 2018 15:02:11	U	SMPL
PB109017BS - 1	LCSW	13174	3.4337	-	7470A	PPB	08 May 2018 15:04:18	U	SMPL
J2759-01 - 1	TP-2	34301	9.0077	-	7470A	PPB	08 May 2018 15:06:25	U	SMPL
J2764-01 - 1	WATER-WELL	6964	1.7953	-	7470A	PPB	08 May 2018 15:08:33	U	SMPL
J2764-01DUP - 1	WATER-WELLDUP	6987	1.8013	-	7470A	PPB	08 May 2018 15:10:44	U	SMPL
J2764-01MS - 1	WATER-WELLS	23753	6.2248	-	7470A	PPB	08 May 2018 15:12:53	U	SMPL
J2764-01MSD - 1	WATER-WELLSMSD	23375	6.1251	-	7470A	PPB	08 May 2018 15:15:00	U	SMPL
CV59 - 1	CCV59	19324	5.0563	-	7470A	PPB	08 May 2018 15:17:08	U	SMPL
CB59 - 1	CCB59	-124	-0.0748	-	7470A	PPB	08 May 2018 15:19:17	U	SMPL
J2675-02LX5 - 1		-88	-0.0653	-	7470A	PPB	08 May 2018 15:21:24	U	SMPL
J2675-02A - 1		13867	3.6165	-	7470A	PPB	08 May 2018 15:23:31	U	SMPL
J2776-02LX5 - 1		-161	-0.0845	-	7470A	PPB	08 May 2018 15:25:38	U	SMPL
J2776-02A - 1		13198	3.4400	-	7470A	PPB	08 May 2018 15:27:46	U	SMPL
J2764-02LX5 - 1		-161	-0.0845	-	7470A	PPB	08 May 2018 15:29:53	U	SMPL
J2764-02A - 1		13339	3.4772	-	7470A	PPB	08 May 2018 15:32:00	U	SMPL
J2764-01A - 1		22591	5.9182	-	7470A	PPB	08 May 2018 15:36:16	U	SMPL
J2764-01LX5 - 1		1328	0.3083	-	7470A	PPB	08 May 2018 15:40:52	U	SMPL
CV60 - 1	CCV60	18726	4.8985	-	7470A	PPB	08 May 2018 15:43:42	U	SMPL
CB60 - 1	CCB60	-90	-0.0658	-	7470A	PPB	08 May 2018 15:45:49	U	SMPL