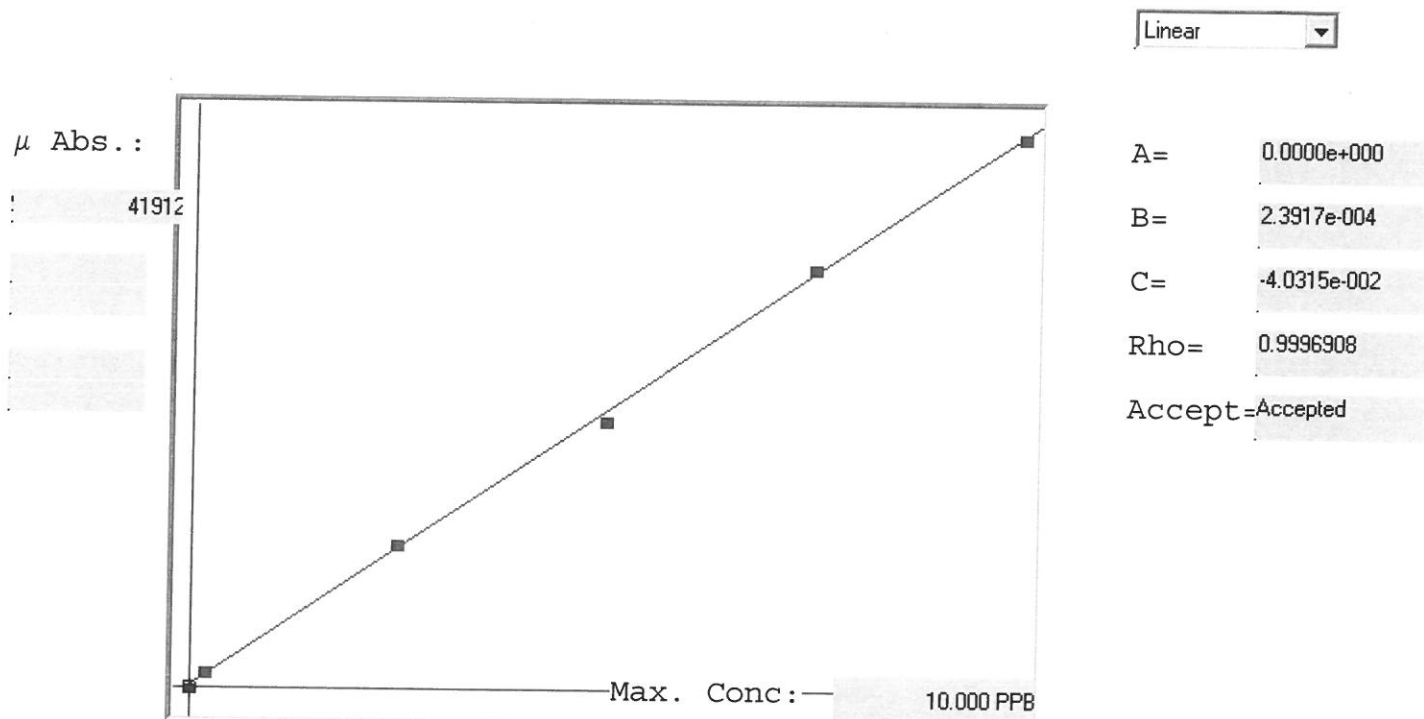


7471B

LB 95201
INSTRUMENT ID: CV1

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.040	-0.040	2	0.000	2				
0.2	0.200	0.249	0.049	1210	0.0 %	1210				
2.5	2.500	2.576	0.076	10941	0.0 %	10941				
5.0	5.000	4.827	-0.173	20352	0.0 %	20352				
7.5	7.500	7.603	0.103	31957	0.0 %	31957				
10.0	10.000	9.984	-0.016	41912	0.0 %	41912				

LB95201 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 08 May 2018 17:16:54

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	2	-	0.0000	7471B	PPB	08 May 2018 17:22:10	S	Std
0.2 - 1	50.2	1210	-	0.2000	7471B	PPB	08 May 2018 17:24:27	S	Std
2.5 - 1	52.5	10941	-	2.5000	7471B	PPB	08 May 2018 17:26:45	S	Std
5.0 - 1	55	20352	-	5.0000	7471B	PPB	08 May 2018 17:29:02	S	Std
7.5 - 1	57.5	31957	-	7.5000	7471B	PPB	08 May 2018 17:31:20	S	Std
10.0 - 1	510	41912	-	10.0000	7471B	PPB	08 May 2018 17:33:37	S	Std
ICV35 - 1	ICV35	16529	3.9130	-7471B	PPB	08 May 2018 17:36:42	U	SMPL	
ICB35 - 1	ICB35	-147	-0.0755	-7471B	PPB	08 May 2018 17:38:57	U	SMPL	
CCV61 - 1	CCV61	21001	4.9826	-7471B	PPB	08 May 2018 17:41:13	U	SMPL	
CCB61 - 1	CCB61	-193	-0.0865	-7471B	PPB	08 May 2018 17:43:29	U	SMPL	
CRA - 1	CRA	1031	0.2063	-7471B	PPB	08 May 2018 17:45:46	U	SMPL	
HighStd - 1	HighStd	42340	10.0863	-7471B	PPB	08 May 2018 17:48:02	U	SMPL	
ChkStd - 1	ChkStd	30896	7.3492	-7471B	PPB	08 May 2018 17:50:18	U	SMPL	
PB109016BL - 1	PBS	-28	-0.0470	-7471B	PPB	08 May 2018 17:52:26	U	SMPL	
PB109016BS - 1	LCSS	15348	3.6305	-7471B	PPB	08 May 2018 17:54:42	U	SMPL	
J2671-01 - 1	AU-02-050718-A	1199	0.2465	-7471B	PPB	08 May 2018 18:06:26	U	SMPL	
J2671-01DUP - 1	AU-02-050718-ADUP	1167	0.2388	-7471B	PPB	08 May 2018 18:10:42	U	SMPL	
J2671-01MS - 1	AU-02-050718-AMS	16135	3.8188	-7471B	PPB	08 May 2018 18:19:59	U	SMPL	
J2671-01MSD - 1	AU-02-050718-AMSD	17049	4.0374	-7471B	PPB	08 May 2018 18:22:16	U	SMPL	
J2671-03 - 1	AU-02-050718-B	1035	0.2072	-7471B	PPB	08 May 2018 18:24:32	U	SMPL	
CCV62 - 1	CCV62	20937	4.9673	-7471B	PPB	08 May 2018 18:26:48	U	SMPL	
CCB62 - 1	CCB62	-146	-0.0752	-7471B	PPB	08 May 2018 18:29:04	U	SMPL	
J2674-01 - 1	HD-02-050718	2354	0.5227	-7471B	PPB	08 May 2018 18:31:21	U	SMPL	
J2676-01 - 1	CL-01-050718-A	1655	0.3555	-7471B	PPB	08 May 2018 18:33:37	U	SMPL	
J2676-03 - 1	CL-01-050718-B	2324	0.5155	-7471B	PPB	08 May 2018 18:35:53	U	SMPL	
J2676-05 - 1	CL-01-050718-C	3000	0.6772	-7471B	PPB	08 May 2018 18:38:09	U	SMPL	
J2676-07 - 1	CL-01-050718-D	4246	0.9752	-7471B	PPB	08 May 2018 18:40:26	U	SMPL	
J2676-09 - 1	CL-01-050718-E	4142	0.9503	-7471B	PPB	08 May 2018 18:42:43	U	SMPL	
J2677-03 - 1	OK-01-050718	941	0.1847	-7471B	PPB	08 May 2018 18:45:01	U	SMPL	
J2759-04 - 1	TP-2A-COMP	8941	2.0981	-7471B	PPB	08 May 2018 18:47:18	U	SMPL	
J2759-07 - 1	TP-2B-COMP	3692	0.8427	-7471B	PPB	08 May 2018 18:49:36	U	SMPL	
J2790-01 - 1	FK-SF-01-004-A	4832	1.1154	-7471B	PPB	08 May 2018 18:51:52	U	SMPL	
CCV63 - 1	CCV63	20769	4.9271	-7471B	PPB	08 May 2018 18:54:08	U	SMPL	
CCB63 - 1	CCB63	-155	-0.0774	-7471B	PPB	08 May 2018 18:56:25	U	SMPL	
J2790-03 - 1	FK-SF-01-004-B	4447	1.0233	-7471B	PPB	08 May 2018 18:58:42	U	SMPL	
J2791-01 - 1	FK-GF-01-004-A	2732	0.6131	-7471B	PPB	08 May 2018 19:00:59	U	SMPL	
J2791-03 - 1	FK-GF-01-004-B	3101	0.7014	-7471B	PPB	08 May 2018 19:03:15	U	SMPL	
J2792-01 - 1	FK-GF-01-003-A	2622	0.5868	-7471B	PPB	08 May 2018 19:05:31	U	SMPL	
J2792-03 - 1	FK-GF-01-003-B	2753	0.6181	-7471B	PPB	08 May 2018 19:07:48	U	SMPL	
J2671-01LX5 - 1		152	-0.0040	-7471B	PPB	08 May 2018 19:10:05	U	SMPL	
J2671-01A - 1		18303	4.3373	-7471B	PPB	08 May 2018 19:12:22	U	SMPL	
CCV64 - 1	CCV64	21100	5.0063	-7471B	PPB	08 May 2018 19:14:40	U	SMPL	
CCB64 - 1	CCB64	-124	-0.0700	-7471B	PPB	08 May 2018 19:16:58	U	SMPL	