

7471B


LB95213

INSTRUMENT ID: CV1

Linear

 μ Abs.:

45161

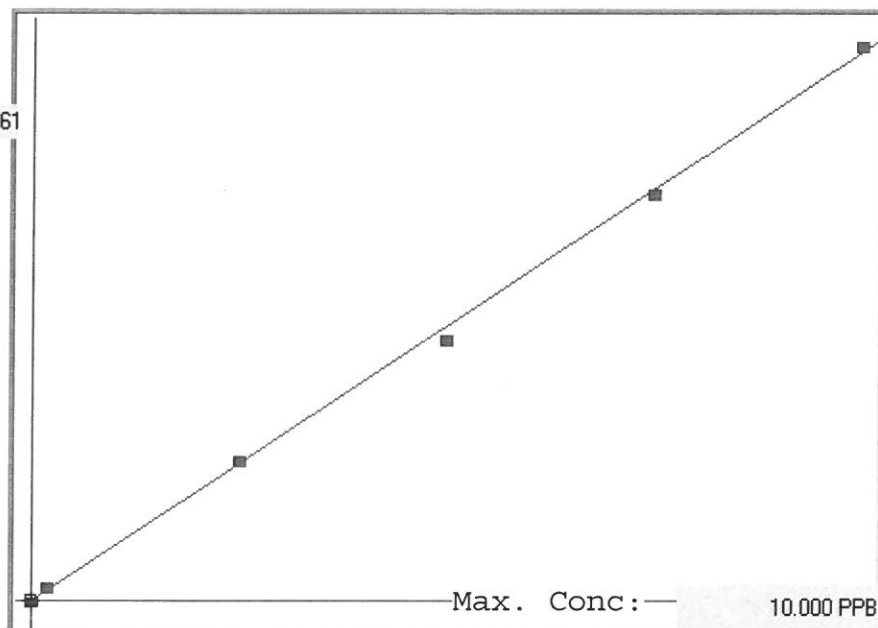

A= 0.0000e+000

B= 2.2385e-004

C= 1.0177e-002

Rho= 0.9995519

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.017	0.017	31	0.000	31				
0.2	0.200	0.257	0.057	1104	0.0 %	1104				
2.5	2.500	2.574	0.074	11453	0.0 %	11453				
5.0	5.000	4.782	-0.218	21318	0.0 %	21318				
7.5	7.500	7.450	-0.050	33238	0.0 %	33238				
10.0	10.000	10.119	0.119	45161	0.0 %	45161				

LB95213 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 09 May 2018 11:09:39

Sample ID	Extended ID	μ Abs.	Conc.	Std ConcMethod	Units	Date	Type	Type
0.0 - 1	5.0	31	-	0.00007471B	PPB	09 May 2018 11:17:21	S	Std
0.2 - 1	50.2	1104	-	0.20007471B	PPB	09 May 2018 11:22:12	S	Std
2.5 - 1	52.5	11453	-	2.50007471B	PPB	09 May 2018 11:24:30	S	Std
5.0 - 1	55	21318	-	5.00007471B	PPB	09 May 2018 11:29:24	S	Std
7.5 - 1	57.5	33238	-	7.50007471B	PPB	09 May 2018 11:31:40	S	Std
10.0 - 1	510	45161	-	10.00007471B	PPB	09 May 2018 11:33:58	S	Std
ICV37 - 1	ICV37	16689	3.7459	-7471B	PPB	09 May 2018 11:37:10	U	SMPL
ICB37 - 1	ICB37	-144	-0.0221	-7471B	PPB	09 May 2018 11:39:25	U	SMPL
CCV71 - 1	CCV71	21733	4.8750	-7471B	PPB	09 May 2018 11:41:41	U	SMPL
CCB71 - 1	CCB71	-125	-0.0178	-7471B	PPB	09 May 2018 11:43:57	U	SMPL
CRA - 1	CRA	1110	0.2586	-7471B	PPB	09 May 2018 11:46:13	U	SMPL
HighStd - 1	HighStd	45463	10.1869	-7471B	PPB	09 May 2018 11:48:29	U	SMPL
ChkStd - 1	ChkStd	29902	6.7036	-7471B	PPB	09 May 2018 11:50:45	U	SMPL
PB109061BL - 1	PBS	-252	-0.0462	-7471B	PPB	09 May 2018 11:53:03	U	SMPL
PB109061BS - 1	LCSS	14743	3.3103	-7471B	PPB	09 May 2018 11:55:22	U	SMPL
J1578-05 - 1	OILY-DEBRIS	-129	-0.0187	-7471B	PPB	09 May 2018 11:57:38	U	SMPL
J1585-02 - 1	FMS-SOIL-1	2473	0.5637	-7471B	PPB	09 May 2018 11:59:56	U	SMPL
J1585-12 - 1	FMS-SOIL-2	1953	0.4473	-7471B	PPB	09 May 2018 12:02:13	U	SMPL
J2669-05 - 1	SU-02-050818	5020	1.1339	-7471B	PPB	09 May 2018 12:04:31	U	SMPL
J2669-05DUP - 1	SU-02-050818DUP	4664	1.0542	-7471B	PPB	09 May 2018 12:06:47	U	SMPL
CCV72 - 1	CCV72	21337	4.7864	-7471B	PPB	09 May 2018 12:09:03	U	SMPL
CCB72 - 1	CCB72	-139	-0.0209	-7471B	PPB	09 May 2018 12:11:19	U	SMPL
J2669-05MS - 1	SU-02-050818MS	20960	4.7020	-7471B	PPB	09 May 2018 12:13:35	U	SMPL
J2669-05MSD - 1	SU-02-050818MSD	19767	4.4349	-7471B	PPB	09 May 2018 12:15:51	U	SMPL
J2780-05 - 1	SOIL	3168	0.7193	-7471B	PPB	09 May 2018 12:18:08	U	SMPL
J2783-01 - 1	BS-CONCRETE-RO-277	64	0.0245	-7471B	PPB	09 May 2018 12:20:25	U	SMPL
J2783-04 - 1	BS-OILY-STONE-RO-208	39	0.0189	-7471B	PPB	09 May 2018 12:22:41	U	SMPL
J2784-01 - 1	RO-160	8688	1.9549	-7471B	PPB	09 May 2018 12:24:58	U	SMPL
J2803-01 - 1	LS-OILY-STONE	610	0.1467	-7471B	PPB	09 May 2018 12:27:16	U	SMPL
J2804-01 - 1	EPE-MX-5(0-5)	5836	1.3165	-7471B	PPB	09 May 2018 12:29:33	U	SMPL
J2804-02 - 1	EPE-MX-5(5-10)	300	0.0773	-7471B	PPB	09 May 2018 12:31:51	U	SMPL
J2804-03 - 1	EPE-116-1(0-5)	2709	0.6166	-7471B	PPB	09 May 2018 12:34:07	U	SMPL
CCV73 - 1	CCV73	21890	4.9101	-7471B	PPB	09 May 2018 12:36:24	U	SMPL
CCB73 - 1	CCB73	-114	-0.0153	-7471B	PPB	09 May 2018 12:38:40	U	SMPL
J2804-04 - 1	EPE-116-1(5-10)	1017	0.2378	-7471B	PPB	09 May 2018 12:40:57	U	SMPL
J2805-01 - 1	WC-11(10-15)D3	2531	0.5767	-7471B	PPB	09 May 2018 12:43:13	U	SMPL
J2805-03 - 1	WC-12(5-10)J4	13407	3.0113	-7471B	PPB	09 May 2018 12:45:29	U	SMPL
J2806-01 - 1	CS-OILY-STONE	-80	-0.0077	-7471B	PPB	09 May 2018 12:47:46	U	SMPL
J2811-02 - 1	TP-4A	5696	1.2852	-7471B	PPB	09 May 2018 12:50:03	U	SMPL
J2811-05 - 1	TP-6A	7589	1.7089	-7471B	PPB	09 May 2018 12:52:20	U	SMPL
J2811-08 - 1	TP-6B	15471	3.4733	-7471B	PPB	09 May 2018 12:54:37	U	SMPL
J2669-05LX5 - 1		850	0.2004	-7471B	PPB	09 May 2018 12:56:55	U	SMPL
J2669-05A - 1		21183	4.7519	-7471B	PPB	09 May 2018 12:59:12	U	SMPL
CCV74 - 1	CCV74	21603	4.8459	-7471B	PPB	09 May 2018 13:01:29	U	SMPL
CCB74 - 1	CCB74	-125	-0.0178	-7471B	PPB	09 May 2018 13:03:45	U	SMPL