


7470A

LB95417
INSTRUMENT ID: CV1

Linear

 μ Abs.:

36380

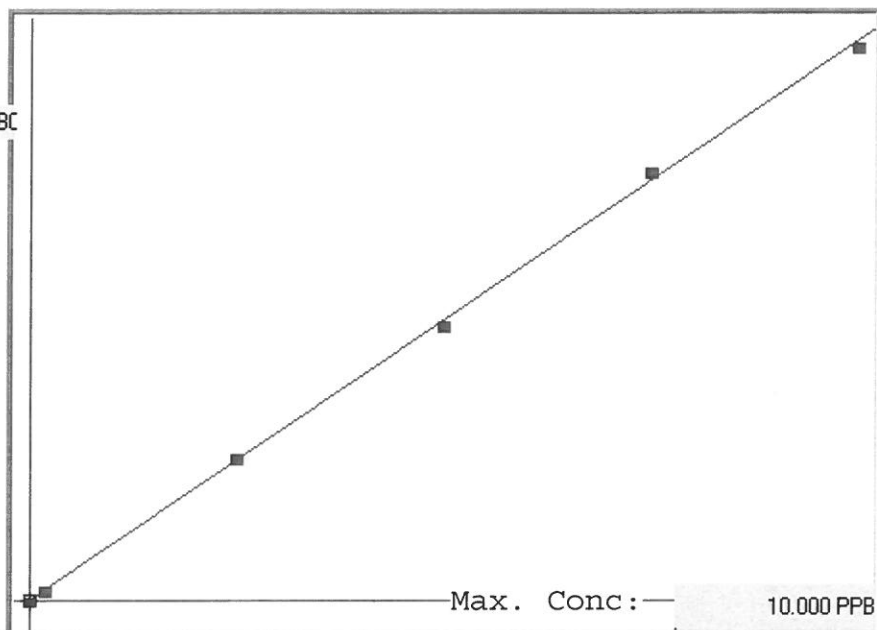

A= 0.0000e+000

B= 2.7231e-004

C= -5.0399e-003

Rho= 0.9997236

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.016	-0.016	-40	0.000	-40				
0.2	0.200	0.191	-0.009	719	0.0 %	719				
2.5	2.500	2.537	0.037	9335	0.0 %	9335				
5.0	5.000	4.921	-0.079	18088	0.0 %	18088				
7.5	7.500	7.666	0.166	28169	0.0 %	28169				
10.0	10.000	9.902	-0.098	36380	0.0 %	36380				

LB95417 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 17 May 2018 13:12:48

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	SC	-40	-	0.0000	7470A	PPB	17 May 2018 13:13:37	S	Std
0.2 - 1	502	719	-	0.2000	7470A	PPB	17 May 2018 13:15:45	S	Std
2.5 - 1	52.5	9335	-	2.5000	7470A	PPB	17 May 2018 13:17:54	S	Std
5.0 - 1	55	18088	-	5.0000	7470A	PPB	17 May 2018 13:20:01	S	Std
7.5 - 1	55.5	28169	-	7.5000	7470A	PPB	17 May 2018 13:22:09	S	Std
10.0 - 1	510	36380	-	10.0000	7470A	PPB	17 May 2018 13:26:47	S	Std
ICV52 - 1	ICV52	15114	4.1107	-	7470A	PPB	17 May 2018 13:34:04	U	SMPL
ICB52 - 1	ICB52	-258	-0.0753	-	7470A	PPB	17 May 2018 13:36:11	U	SMPL
CCV71 - 1	CCV71	17977	4.8904	-	7470A	PPB	17 May 2018 13:38:19	U	SMPL
CCB71 - 1	CCB71	-219	-0.0647	-	7470A	PPB	17 May 2018 13:40:25	U	SMPL
CRA - 1	CRA	724	0.1921	-	7470A	PPB	17 May 2018 13:42:33	U	SMPL
HighStd - 1	HighStd	36432	9.9159	-	7470A	PPB	17 May 2018 13:44:40	U	SMPL
ChkStd - 1	ChkStd	24204	6.5861	-	7470A	PPB	17 May 2018 13:53:30	U	SMPL
PB109386BL - 1	PBW	-302	-0.0873	-	7470A	PPB	17 May 2018 13:55:36	U	SMPL
PB109386BS - 1	LCSW	13824	3.7594	-	7470A	PPB	17 May 2018 13:57:46	U	SMPL
J2519-02 - 1	OILY-WATER-TOTE	-310	-0.0895	-	7470A	PPB	17 May 2018 13:59:53	U	SMPL
J2930-01 - 1	MW01	-153	-0.0467	-	7470A	PPB	17 May 2018 14:02:02	U	SMPL
J2943-01 - 1	MW-10	-111	-0.0353	-	7470A	PPB	17 May 2018 14:04:10	U	SMPL
J2943-01DUP - 1	MW-10DUP	-100	-0.0323	-	7470A	PPB	17 May 2018 14:06:19	U	SMPL
J2943-01MS - 1	MW-10MS	12816	3.4849	-	7470A	PPB	17 May 2018 14:08:25	U	SMPL
CCV72 - 1	CCV72	17943	4.8811	-	7470A	PPB	17 May 2018 14:10:32	U	SMPL
CCB72 - 1	CCB72	-237	-0.0696	-	7470A	PPB	17 May 2018 14:12:39	U	SMPL
J2943-01MSD - 1	MW-10MSD	12795	3.4792	-	7470A	PPB	17 May 2018 14:14:48	U	SMPL
J2943-02 - 1	MW-1	388	0.1006	-	7470A	PPB	17 May 2018 14:16:54	U	SMPL
J2943-03 - 1	MW-D	-139	-0.0429	-	7470A	PPB	17 May 2018 14:19:02	U	SMPL
J2966-09 - 1	BUR-DRUM-1-TREN-DRUM-1	506	0.1328	-	7470A	PPB	17 May 2018 14:21:09	U	SMPL
J2943-01LX5 - 1		-102	-0.0328	-	7470A	PPB	17 May 2018 14:23:17	U	SMPL
J2943-01A - 1		14041	3.8185	-	7470A	PPB	17 May 2018 14:25:24	U	SMPL
CCV73 - 1	CCV73	17564	4.7779	-	7470A	PPB	17 May 2018 14:27:32	U	SMPL
CCB73 - 1	CCB73	-167	-0.0505	-	7470A	PPB	17 May 2018 14:29:42	U	SMPL