


L395837

7470A

INSTRUMENT ID: CX2

Linear

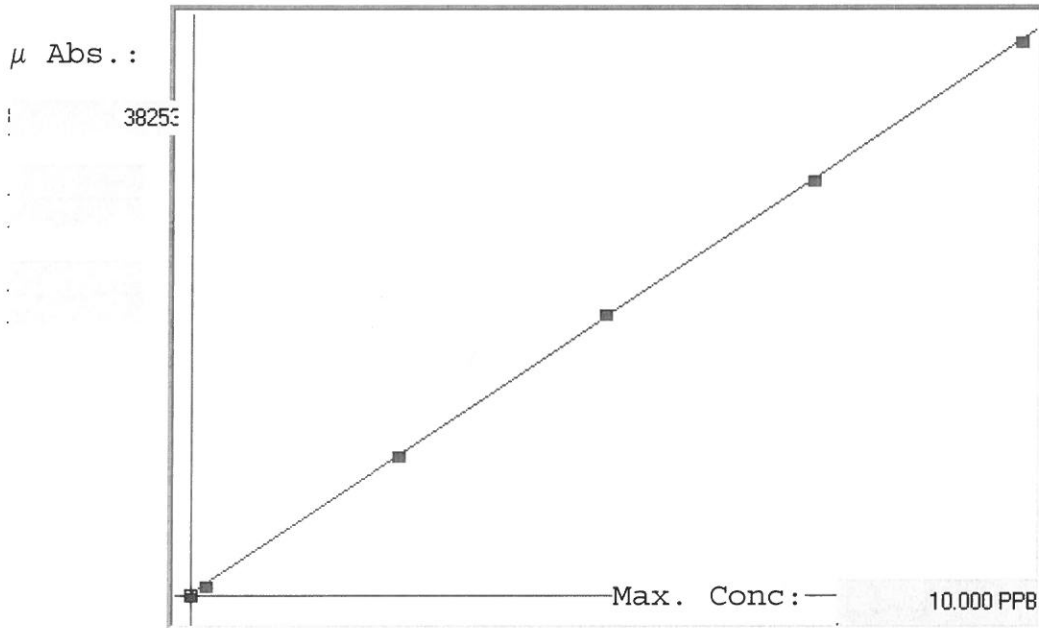

A= 0.0000e+000

B= 2.6125e-004

C= -2.5632e-002

Rho= 0.9999565

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.011	-0.011	55	0.000	55				
0.2	0.200	0.176	-0.024	771	0.0 %	771				
2.5	2.500	2.501	0.001	9672	0.0 %	9672				
5.0	5.000	5.073	0.073	19516	0.0 %	19516				
7.5	7.500	7.493	-0.007	28780	0.0 %	28780				
10.0	10.000	9.968	-0.032	38253	0.0 %	38253				

LB95837 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 06 Jun 2018 11:20:03

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	55	-	0.0000	7470A	PPB	06 Jun 2018 11:25:31	S	Std
0.2 - 1	50.2	771	-	0.2000	7470A	PPB	06 Jun 2018 11:27:39	S	Std
2.5 - 1	52.5	9672	-	2.5000	7470A	PPB	06 Jun 2018 11:29:47	S	Std
5.0 - 1	55	19516	-	5.0000	7470A	PPB	06 Jun 2018 11:31:55	S	Std
7.5 - 1	57.5	28780	-	7.5000	7470A	PPB	06 Jun 2018 11:34:03	S	Std
10.0 - 1	510	38253	-	10.0000	7470A	PPB	06 Jun 2018 11:36:11	S	Std
ICV85 - 1	ICV85	15069	3.9112	-	7470A	PPB	06 Jun 2018 11:38:45	U	SMPL
ICB85 - 1	ICB85	-129	-0.0593	-	7470A	PPB	06 Jun 2018 11:40:51	U	SMPL
CCV61 - 1	CCV61	19619	5.0999	-	7470A	PPB	06 Jun 2018 11:42:57	U	SMPL
CCB61 - 1	CCB61	-87	-0.0484	-	7470A	PPB	06 Jun 2018 11:45:04	U	SMPL
CRA - 1	CRA	750	0.1703	-	7470A	PPB	06 Jun 2018 11:47:11	U	SMPL
HighStd - 1	HighStd	38581	10.0538	-	7470A	PPB	06 Jun 2018 11:49:17	U	SMPL
ChkStd - 1	ChkStd	26317	6.8498	-	7470A	PPB	06 Jun 2018 11:51:24	U	SMPL
PB109995BL - 1	PBW	-176	-0.0716	-	7470A	PPB	06 Jun 2018 11:53:33	U	SMPL
PB109995BS - 1	LCSW	13777	3.5736	-	7470A	PPB	06 Jun 2018 11:55:42	U	SMPL
PB109995TB - 1	PB109958TB	-79	-0.0463	-	7470A	PPB	06 Jun 2018 11:57:49	U	SMPL
J2309-06 - 1	ROCKY-SOIL	12	-0.0225	-	7470A	PPB	06 Jun 2018 11:59:58	U	SMPL
J2309-10 - 1	OILY-CONCRETE	13	-0.0222	-	7470A	PPB	06 Jun 2018 12:02:06	U	SMPL
J3195-11 - 1	OILY-STONES	38	-0.0157	-	7470A	PPB	06 Jun 2018 12:04:14	U	SMPL
J3195-11DUP - 1	OILY-STONESDUP	37	-0.0160	-	7470A	PPB	06 Jun 2018 12:06:21	U	SMPL
CCV62 - 1	CCV62	19245	5.0022	-	7470A	PPB	06 Jun 2018 12:08:27	U	SMPL
CCB62 - 1	CCB62	-100	-0.0518	-	7470A	PPB	06 Jun 2018 12:10:34	U	SMPL
J3195-11MS - 1	OILY-STONESMS	13953	3.6196	-	7470A	PPB	06 Jun 2018 12:12:42	U	SMPL
J3195-11MSD - 1	OILY-STONESMSD	14491	3.7602	-	7470A	PPB	06 Jun 2018 12:14:48	U	SMPL
J3300-04 - 1	ROCKPILE-SANDPILE	-144	-0.0633	-	7470A	PPB	06 Jun 2018 12:16:56	U	SMPL
J3304-03 - 1	FS-SOIL	25	-0.0191	-	7470A	PPB	06 Jun 2018 12:19:04	U	SMPL
J3304-06 - 1	FS-CON	10	-0.0230	-	7470A	PPB	06 Jun 2018 12:21:11	U	SMPL
J3305-06 - 1	DRUM-1-DRUM-2-ROCKS	13	-0.0222	-	7470A	PPB	06 Jun 2018 12:23:18	U	SMPL
J3305-07 - 1	DRUM-1-DRUM-2-WIPES	74	-0.0063	-	7470A	PPB	06 Jun 2018 12:25:27	U	SMPL
J3306-01 - 1	AM-SOIL	32	-0.0173	-	7470A	PPB	06 Jun 2018 12:27:35	U	SMPL
PB109996BL - 1	PBW	18	-0.0209	-	7470A	PPB	06 Jun 2018 12:29:43	U	SMPL
PB109996BS - 1	LCSW	13846	3.5917	-	7470A	PPB	06 Jun 2018 12:31:50	U	SMPL
CCV63 - 1	CCV63	19082	4.9596	-	7470A	PPB	06 Jun 2018 12:33:57	U	SMPL
CCB63 - 1	CCB63	-125	-0.0583	-	7470A	PPB	06 Jun 2018 12:36:04	U	SMPL
PB109996TB - 1	PB109962TB	13	-0.0222	-	7470A	PPB	06 Jun 2018 12:38:12	U	SMPL
J3306-03 - 1	AM-WATER	62	-0.0094	-	7470A	PPB	06 Jun 2018 12:40:19	U	SMPL
J3306-03DUP - 1	AM-WATERDUP	128	0.0078	-	7470A	PPB	06 Jun 2018 12:42:26	U	SMPL
J3306-03MS - 1	AM-WATERMS	13176	3.4166	-	7470A	PPB	06 Jun 2018 12:44:33	U	SMPL
J3306-03MSD - 1	AM-WATERMSD	13272	3.4417	-	7470A	PPB	06 Jun 2018 12:46:40	U	SMPL
J3195-11LX5 - 1		-103	-0.0525	-	7470A	PPB	06 Jun 2018 12:48:48	U	SMPL
J3195-11A - 1		14300	3.7103	-	7470A	PPB	06 Jun 2018 12:50:57	U	SMPL
J3306-03LX5 - 1		-83	-0.0473	-	7470A	PPB	06 Jun 2018 12:53:05	U	SMPL
J3306-03A - 1		13251	3.4362	-	7470A	PPB	06 Jun 2018 12:55:14	U	SMPL
CCV64 - 1	CCV64	18836	4.8953	-	7470A	PPB	06 Jun 2018 12:57:21	U	SMPL
CCB64 - 1	CCB64	-112	-0.0549	-	7470A	PPB	06 Jun 2018 12:59:30	U	SMPL