

1395839

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

6/6/2018 12:43

Test: ^{Reactive} ~~Total~~ CN ^{Mg/d}

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	97.496	0.0	0.096	
ICB1	-0.315	0.0	0.004	
CCV1	242.973	0.0	0.233	
CCB1	0.057	0.0	0.004	
PB110007BL	-0.315	0.0	0.004	
J3241-02	-0.353	0.0	0.004	
J3241-02DUP	-0.110	0.0	0.004	
J3241-04	-0.346	0.0	0.004	
J3241-06	-0.245	0.0	0.004	
J3325-02	-0.415	0.0	0.003	
J3326-03	-0.402	0.0	0.003	
J3251-02	-0.436	0.0	0.003	
CCV2	266.945	0.0	0.256	
CCB2	-0.504	0.0	0.003	

N 14
Mean 43.145
SD 93.5378
CV% 216.80

AS

Aquakem v. 7.2AQ1

Results from time period:

Wed Jun 06 11:39:56 2018

Wed Jun 06 12:41:35 2018

Sample Id	Sam/Ctr/c	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Total CN	P	-0.5998	µg/l	6/6/2018 11:39:56	
5.0PPBCN	A	Total CN	P	4.5818	µg/l	6/6/2018 11:39:57	
10PPBCN	A	Total CN	P	10.0549	µg/l	6/6/2018 11:39:58	
50PPBCN	A	Total CN	P	50.15	µg/l	6/6/2018 11:39:59	
100PPBCN	A	Total CN	P	100.2317	µg/l	6/6/2018 11:40:00	
250PPBCN	A	Total CN	P	251.2793	µg/l	6/6/2018 11:40:01	
500PPBCN	A	Total CN	P	499.3021	µg/l	6/6/2018 11:40:02	
ICV1	S	Total CN	P	97.4964	µg/l	6/6/2018 12:14:15	
ICB1	S	Total CN	P	-0.3153	µg/l	6/6/2018 12:14:16	
CCV1	S	Total CN	P	242.9725	µg/l	6/6/2018 12:14:17	
CCB1	S	Total CN	P	0.0567	µg/l	6/6/2018 12:14:18	
PB110007BL	S	Total CN	P	-0.3147	µg/l	6/6/2018 12:14:19	
J3241-02	S	Total CN	P	-0.3531	µg/l	6/6/2018 12:14:20	
J3241-02DUP	S	Total CN	P	-0.1102	µg/l	6/6/2018 12:14:21	
J3241-04	S	Total CN	P	-0.3456	µg/l	6/6/2018 12:14:22	
J3241-06	S	Total CN	P	-0.2451	µg/l	6/6/2018 12:14:23	
J3325-02	S	Total CN	P	-0.4146	µg/l	6/6/2018 12:14:25	
J3326-03	S	Total CN	P	-0.4016	µg/l	6/6/2018 12:18:06	
J3251-02	S	Total CN	P	-0.4358	µg/l	6/6/2018 12:41:33	
CCV2	S	Total CN	P	266.9452	µg/l	6/6/2018 12:41:34	
CCB2	S	Total CN	P	-0.504	µg/l	6/6/2018 12:41:35	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

6/6/2018 11:49


Test Total CN

Accepted 6/6/2018 11:49

Factor 1059
Bias 0.004

Coeff. of det. 0.999987

Errors

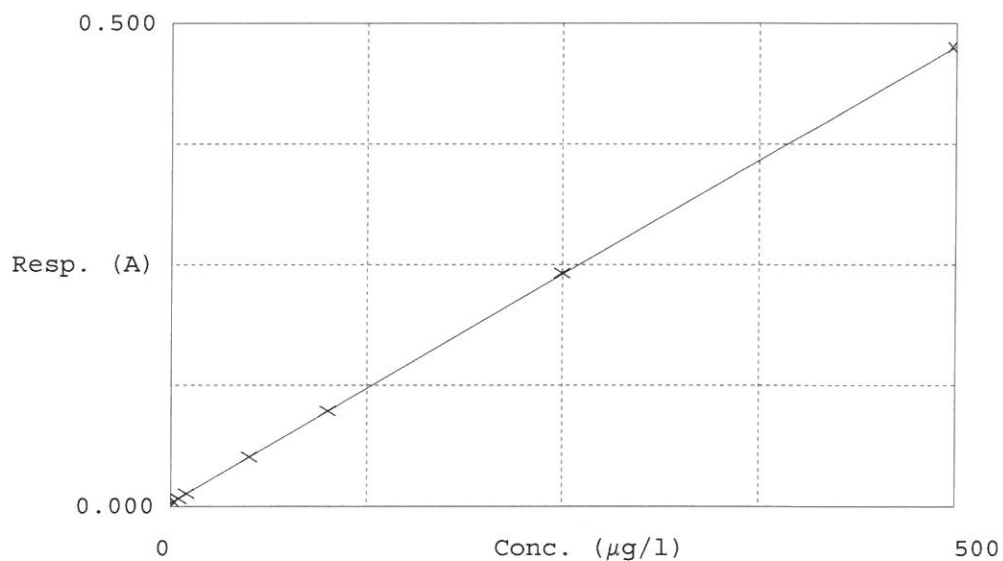

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.003	-0.5998	0.0000	
2	5.0PPBCN	0.008	4.5818	5.0000	
3	10PPBCN	0.013	10.0549	10.0000	
4	50PPBCN	0.051	50.1500	50.0000	
5	100PPBCN	0.099	100.2317	100.0000	
6	250PPBCN	0.241	251.2793	250.0000	
7	500PPBCN	0.476	499.3021	500.0000	