

7470A


LB95998

INSTRUMENT ID: CV1

Linear

 μ Abs.:

37952

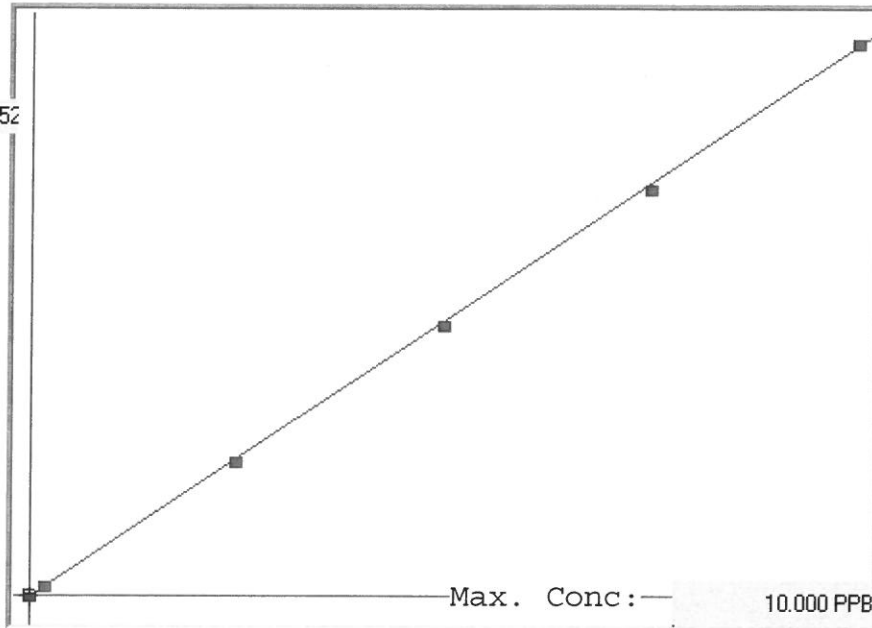

A= 0.0000e+000

B= 2.6486e-004

C= 2.8642e-002

Rho= 0.9999025

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.027	0.027	-6	0.000	-6				
0.2	0.200	0.222	0.022	731	0.0 %	731				
2.5	2.500	2.489	-0.011	9290	0.0 %	9290				
5.0	5.000	4.962	-0.038	18628	0.0 %	18628				
7.5	7.500	7.418	-0.082	27900	0.0 %	27900				
10.0	10.000	10.081	0.081	37952	0.0 %	37952				

LB95998 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 14 Jun 2018 10:30:29

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-6	-	0.0000	7470A	PPB	14 Jun 2018 10:43:16	S	Std
0.2 - 1	50.2	731	-	0.2000	7470A	PPB	14 Jun 2018 10:45:24	S	Std
2.5 - 1	52.5	9290	-	2.5000	7470A	PPB	14 Jun 2018 10:47:32	S	Std
5.0 - 1	55	18628	-	5.0000	7470A	PPB	14 Jun 2018 10:49:40	S	Std
7.5 - 1	57.5	27900	-	7.5000	7470A	PPB	14 Jun 2018 10:51:48	S	Std
10.0 - 1	510	37952	-	10.0000	7470A	PPB	14 Jun 2018 10:53:56	S	Std
ICV01 - 1	ICV01	13604	3.6318	-7470A	PPB	PPB	14 Jun 2018 10:56:32	U	SMPL
ICB01 - 1	ICB01	-123	-0.0039	-7470A	PPB	PPB	14 Jun 2018 10:58:38	U	SMPL
CCV23 - 1	CCV23	18202	4.8497	-7470A	PPB	PPB	14 Jun 2018 11:00:45	U	SMPL
CCB23 - 1	CCB23	-115	-0.0018	-7470A	PPB	PPB	14 Jun 2018 11:02:51	U	SMPL
CRA - 1	CRA	743	0.2254	-7470A	PPB	PPB	14 Jun 2018 11:04:59	U	SMPL
HighStd - 1	HighStd	37379	9.9289	-7470A	PPB	PPB	14 Jun 2018 11:07:05	U	SMPL
ChkStd - 1	ChkStd	25586	6.8054	-7470A	PPB	PPB	14 Jun 2018 11:09:12	U	SMPL
PB110217BL - 1	PBW	-161	-0.0140	-7470A	PPB	PPB	14 Jun 2018 11:11:21	U	SMPL
PB110217BS - 1	LCSW	13859	3.6994	-7470A	PPB	PPB	14 Jun 2018 11:13:30	U	SMPL
PB110217TB - 1	PB110189TB	-76	0.0085	-7470A	PPB	PPB	14 Jun 2018 11:15:37	U	SMPL
J3246-02 - 1	OK-02-061218	15	0.0326	-7470A	PPB	PPB	14 Jun 2018 11:17:45	U	SMPL
J3246-02DUP - 1	OK-02-061218DUP	-1	0.0284	-7470A	PPB	PPB	14 Jun 2018 11:19:54	U	SMPL
J3246-02MS - 1	OK-02-061218MS	13719	3.6623	-7470A	PPB	PPB	14 Jun 2018 11:22:02	U	SMPL
J3246-02MSD - 1	OK-02-061218MSD	13885	3.7063	-7470A	PPB	PPB	14 Jun 2018 11:24:09	U	SMPL
CCV24 - 1	CCV24	18109	4.8250	-7470A	PPB	PPB	14 Jun 2018 11:26:16	U	SMPL
CCB24 - 1	CCB24	-129	-0.0055	-7470A	PPB	PPB	14 Jun 2018 11:28:22	U	SMPL
J3251-04 - 1	SU-03-061118	12	0.0318	-7470A	PPB	PPB	14 Jun 2018 11:30:30	U	SMPL
J3459-02 - 1	MH-RO-341	38	0.0387	-7470A	PPB	PPB	14 Jun 2018 11:32:37	U	SMPL
PB110218BL - 1	PBW	10	0.0313	-7470A	PPB	PPB	14 Jun 2018 11:34:43	U	SMPL
PB110218BS - 1	LCSW	14516	3.8734	-7470A	PPB	PPB	14 Jun 2018 11:36:50	U	SMPL
PB110218TB - 1	PB110202TB	-103	0.0014	-7470A	PPB	PPB	14 Jun 2018 11:38:57	U	SMPL
J3448-02 - 1	N-48971	35	0.0379	-7470A	PPB	PPB	14 Jun 2018 11:41:05	U	SMPL
J3448-02DUP - 1	N-48971DUP	28	0.0361	-7470A	PPB	PPB	14 Jun 2018 11:43:13	U	SMPL
J3448-02MS - 1	N-48971MS	14176	3.7833	-7470A	PPB	PPB	14 Jun 2018 11:45:22	U	SMPL
J3448-02MSD - 1	N-48971MSD	13902	3.7108	-7470A	PPB	PPB	14 Jun 2018 11:47:30	U	SMPL
J3448-04 - 1	N-48969	-69	0.0104	-7470A	PPB	PPB	14 Jun 2018 11:49:37	U	SMPL
CCV25 - 1	CCV25	18028	4.8036	-7470A	PPB	PPB	14 Jun 2018 11:51:44	U	SMPL
CCB25 - 1	CCB25	-124	-0.0042	-7470A	PPB	PPB	14 Jun 2018 11:53:51	U	SMPL
J3448-06 - 1	N-48966	15	0.0326	-7470A	PPB	PPB	14 Jun 2018 11:55:59	U	SMPL
J3451-02 - 1	VB-25830-SLUDGEBOX	173	0.0745	-7470A	PPB	PPB	14 Jun 2018 11:58:06	U	SMPL
J3451-04 - 1	VB-44949-SLUDGEBOX	30	0.0366	-7470A	PPB	PPB	14 Jun 2018 12:00:13	U	SMPL
J3456-02 - 1	ES-OILY-WATER	84	0.0509	-7470A	PPB	PPB	14 Jun 2018 12:02:20	U	SMPL
PB110222BL - 1	PBW	3	0.0294	-7470A	PPB	PPB	14 Jun 2018 12:04:27	U	SMPL
PB110222BS - 1	LCSW	13672	3.6498	-7470A	PPB	PPB	14 Jun 2018 12:06:34	U	SMPL
J3448-01 - 1	N-48971	146	0.0673	-7470A	PPB	PPB	14 Jun 2018 12:08:41	U	SMPL
J3448-03 - 1	N-48969	105	0.0565	-7470A	PPB	PPB	14 Jun 2018 12:10:50	U	SMPL
J3448-05 - 1	N-48966	10114	2.7075	-7470A	PPB	PPB	14 Jun 2018 12:12:59	U	SMPL
J3451-01 - 1	VB-25830-SLUDGEBOX	125055	33.1510	-7470A	PPB	PPB	14 Jun 2018 12:15:06	U	SMPL
CCV26 - 1	CCV26	17420	4.6425	-7470A	PPB	PPB	14 Jun 2018 12:17:14	U	SMPL
CCB26 - 1	CCB26	-197	-0.0235	-7470A	PPB	PPB	14 Jun 2018 12:19:29	U	SMPL
J3451-03 - 1	VB-44949-SLUDGEBOX	1370	0.3915	-7470A	PPB	PPB	14 Jun 2018 12:21:37	U	SMPL
J3456-01 - 1	ES-OILY-WATER	1471	0.4183	-7470A	PPB	PPB	14 Jun 2018 12:23:44	U	SMPL
J3456-01DUP - 1	ES-OILY-WATERDUP	1410	0.4021	-7470A	PPB	PPB	14 Jun 2018 12:25:51	U	SMPL
J3456-01MS - 1	ES-OILY-WATERMS	13632	3.6392	-7470A	PPB	PPB	14 Jun 2018 12:30:23	U	SMPL
J3456-01MSD - 1	ES-OILY-WATERMSD	13940	3.7208	-7470A	PPB	PPB	14 Jun 2018 12:32:30	U	SMPL
CCV27 - 1	CCV27	17579	4.6847	-7470A	PPB	PPB	14 Jun 2018 12:34:40	U	SMPL
CCB27 - 1	CCB27	-157	-0.0129	-7470A	PPB	PPB	14 Jun 2018 12:36:49	U	SMPL
J3246-02LX5 - 1		-15	0.0247	-7470A	PPB	PPB	14 Jun 2018 12:38:58	U	SMPL
J3246-02A - 1		14728	3.9295	-7470A	PPB	PPB	14 Jun 2018 12:41:07	U	SMPL
J3448-02LX5 - 1		-100	0.0022	-7470A	PPB	PPB	14 Jun 2018 12:43:13	U	SMPL
J3448-02A - 1		14566	3.8866	-7470A	PPB	PPB	14 Jun 2018 12:45:21	U	SMPL
J3456-01LX5 - 1		285	0.1041	-7470A	PPB	PPB	14 Jun 2018 12:47:28	U	SMPL
J3456-01A - 1		14326	3.8231	-7470A	PPB	PPB	14 Jun 2018 12:52:10	U	SMPL
J3451-01DLX5 - 1		25854	6.8764	-7470A	PPB	PPB	14 Jun 2018 12:54:16	U	SMPL
CCV28 - 1	CCV28	17629	4.6979	-7470A	PPB	PPB	14 Jun 2018 12:56:25	U	SMPL
CCB28 - 1	CCB28	-124	-0.0042	-7470A	PPB	PPB	14 Jun 2018 12:58:34	U	SMPL