

LB 96036


7470A

INSTRUMENT ID: CV1

Linear

μ Abs.:

35584

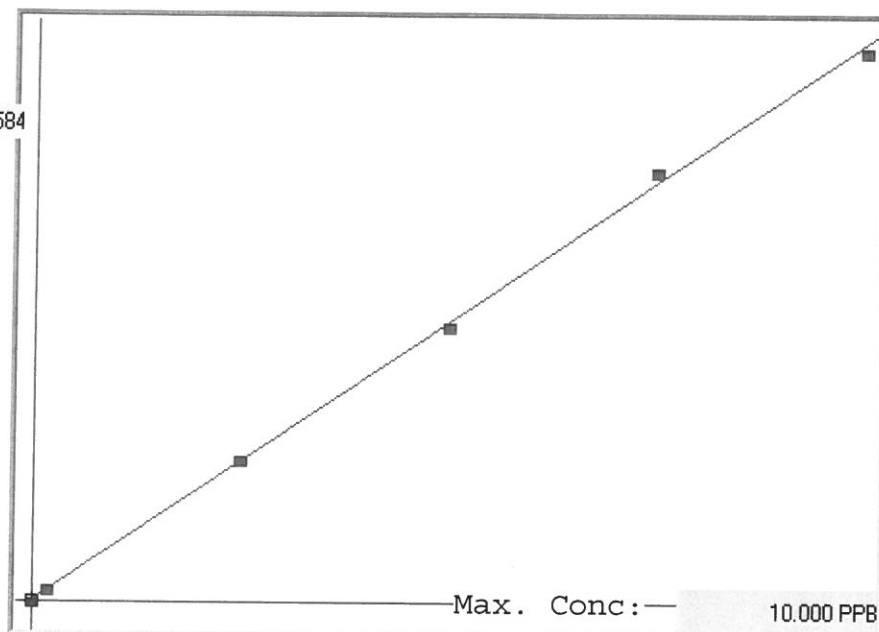

A= 0.0000e+000

B= 2.7802e-004

C= -1.5921e-002

Rho= 0.9996279

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.023	-0.023	-27	0.000	-27				
0.2	0.200	0.194	-0.006	756	0.0 %	756				
2.5	2.500	2.532	0.032	9166	0.0 %	9166				
5.0	5.000	4.924	-0.076	17767	0.0 %	17767				
7.5	7.500	7.696	0.196	27737	0.0 %	27737				
10.0	10.000	9.877	-0.123	35584	0.0 %	35584				

LB96036 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 15 Jun 2018 11:17:04

Sample ID	Extended ID	µ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-27	-	0.00007470A	PPB		15 Jun 2018 11:18:38	S	
0.2 - 1	50.2	756	-	0.20007470A	PPB		15 Jun 2018 11:20:46	S	Std
2.5 - 1	52.5	9166	-	2.50007470A	PPB		15 Jun 2018 11:22:54	S	Std
5.0 - 1	55	17767	-	5.00007470A	PPB		15 Jun 2018 11:25:03	S	Std
7.5 - 1	57.5	27737	-	7.50007470A	PPB		15 Jun 2018 11:27:11	S	Std
10.0 - 1	510	35584	-	10.00007470A	PPB		15 Jun 2018 11:29:18	S	Std
ICV04 - 1	ICV04	13859	3.8372	-7470A	PPB		15 Jun 2018 11:32:00	U	SMPL
ICB04 - 1	ICB04	-164	-0.0615	-7470A	PPB		15 Jun 2018 11:34:06	U	SMPL
CCV39 - 1	CCV39	17712	4.9085	-7470A	PPB		15 Jun 2018 11:36:14	U	SMPL
CCB39 - 1	CCB39	-163	-0.0612	-7470A	PPB		15 Jun 2018 11:38:21	U	SMPL
CRA - 1	CRA	768	0.1976	-7470A	PPB		15 Jun 2018 11:40:28	U	SMPL
HighStd - 1	HighStd	36265	10.0666	-7470A	PPB		15 Jun 2018 11:42:34	U	SMPL
ChkStd - 1	ChkStd	25529	7.0818	-7470A	PPB		15 Jun 2018 11:44:41	U	SMPL
PB110253BL - 1	PBW	-208	-0.0738	-7470A	PPB		15 Jun 2018 11:46:50	U	SMPL
PB110253BS - 1	LCSW	13727	3.8005	-7470A	PPB		15 Jun 2018 11:48:59	U	SMPL
PB110253TB - 1	PB110226TB	-97	-0.0429	-7470A	PPB		15 Jun 2018 11:51:07	U	SMPL
J3239-10 - 1	AU-06-061318-A	-9	-0.0184	-7470A	PPB		15 Jun 2018 11:53:15	U	SMPL
J3239-10DUP - 1	AU-06-061318-ADUP	4	-0.0148	-7470A	PPB		15 Jun 2018 11:55:23	U	SMPL
J3239-10MS - 1	AU-06-061318-AMS	13580	3.7597	-7470A	PPB		15 Jun 2018 11:57:31	U	SMPL
J3239-10MSD - 1	AU-06-061318-AMSD	14299	3.9596	-7470A	PPB		15 Jun 2018 11:59:38	U	SMPL
CCV40 - 1	CCV40	17747	4.9182	-7470A	PPB		15 Jun 2018 12:01:45	U	SMPL
CCB40 - 1	CCB40	-181	-0.0662	-7470A	PPB		15 Jun 2018 12:03:52	U	SMPL
J3239-12 - 1	AU-06-061318-B	-14	-0.0198	-7470A	PPB		15 Jun 2018 12:05:59	U	SMPL
J3239-14 - 1	AU-06-061318-C	6	-0.0143	-7470A	PPB		15 Jun 2018 12:08:06	U	SMPL
J3241-08 - 1	HR-05-061318-A	6	-0.0143	-7470A	PPB		15 Jun 2018 12:10:13	U	SMPL
J3241-10 - 1	HR-05-061318-B	29	-0.0079	-7470A	PPB		15 Jun 2018 12:12:20	U	SMPL
J3241-12 - 1	HR-05-061318-C	36	-0.0059	-7470A	PPB		15 Jun 2018 12:14:27	U	SMPL
J3465-02 - 1	TP-A1-WC-1	-16	-0.0204	-7470A	PPB		15 Jun 2018 12:16:34	U	SMPL
J3465-04 - 1	TP-A2-WC-1	0	-0.0159	-7470A	PPB		15 Jun 2018 12:18:43	U	SMPL
J3465-06 - 1	TP-B4-WC-1	11	-0.0129	-7470A	PPB		15 Jun 2018 12:20:51	U	SMPL
J3480-04 - 1	OILY-STONES	15	-0.0118	-7470A	PPB		15 Jun 2018 12:22:59	U	SMPL
J3487-02 - 1	OILY-SOIL	21	-0.0101	-7470A	PPB		15 Jun 2018 12:25:06	U	SMPL
CCV41 - 1	CCV41	17814	4.9368	-7470A	PPB		15 Jun 2018 12:27:14	U	SMPL
CCB41 - 1	CCB41	-155	-0.0590	-7470A	PPB		15 Jun 2018 12:29:20	U	SMPL
J3488-03 - 1	FS-RO-3091	4	-0.0148	-7470A	PPB		15 Jun 2018 12:31:28	U	SMPL
J3490-04 - 1	CONCRETE-BASE	6	-0.0143	-7470A	PPB		15 Jun 2018 12:33:35	U	SMPL
J3493-02 - 1	WC-1	-2	-0.0165	-7470A	PPB		15 Jun 2018 12:35:42	U	SMPL
PB110256BL - 1	PBW	2	-0.0154	-7470A	PPB		15 Jun 2018 12:37:50	U	SMPL
PB110256BS - 1	LCSW	14008	3.8786	-7470A	PPB		15 Jun 2018 12:39:57	U	SMPL
PB110256TB - 1	PB110251TB	-81	-0.0384	-7470A	PPB		15 Jun 2018 12:42:04	U	SMPL
J3469-02 - 1	OILY-WATER	16	-0.0115	-7470A	PPB		15 Jun 2018 12:44:12	U	SMPL
J3469-02DUP - 1	OILY-WATERDUP	8	-0.0137	-7470A	PPB		15 Jun 2018 12:46:21	U	SMPL
J3469-02MS - 1	OILY-WATERMS	13306	3.6835	-7470A	PPB		15 Jun 2018 12:48:30	U	SMPL
J3469-02MSD - 1	OILY-WATERMSD	12822	3.5489	-7470A	PPB		15 Jun 2018 12:50:37	U	SMPL
CCV42 - 1	CCV42	17703	4.9060	-7470A	PPB		15 Jun 2018 12:52:44	U	SMPL
CCB42 - 1	CCB42	-184	-0.0671	-7470A	PPB		15 Jun 2018 12:54:52	U	SMPL
PB110260BL - 1	PBW	-31	-0.0245	-7470A	PPB		15 Jun 2018 12:57:01	U	SMPL
PB110260BS - 1	LCSW	13972	3.8686	-7470A	PPB		15 Jun 2018 12:59:08	U	SMPL
J3469-01 - 1	OILY-WATER	8786	2.4268	-7470A	PPB		15 Jun 2018 13:01:15	U	SMPL
J3469-01DUP - 1	OILY-WATERDUP	9226	2.5491	-7470A	PPB		15 Jun 2018 13:03:22	U	SMPL
J3469-01MS - 1	OILY-WATERMS	21700	6.0172	-7470A	PPB		15 Jun 2018 13:10:40	U	SMPL
J3469-01MSD - 1	OILY-WATERMSD	21919	6.0781	-7470A	PPB		15 Jun 2018 13:12:48	U	SMPL
J3497-01 - 1	CAS1-WC-L-01	29067	8.0654	-7470A	PPB		15 Jun 2018 13:14:58	U	SMPL
J3502-01 - 1	20180367-SITE-WATER	2324	0.6302	-7470A	PPB		15 Jun 2018 13:17:08	U	SMPL
J3502-02 - 1	20180366-FIELD-BLANK	54	-0.0009	-7470A	PPB		15 Jun 2018 13:19:18	U	SMPL
CCV43 - 1	CCV43	17845	4.9454	-7470A	PPB		15 Jun 2018 13:21:25	U	SMPL
CCB43 - 1	CCB43	-126	-0.0510	-7470A	PPB		15 Jun 2018 13:23:33	U	SMPL
J3239-10LX5 - 1		-19	-0.0212	-7470A	PPB		15 Jun 2018 13:25:41	U	SMPL
J3239-10A - 1		14760	4.0877	-7470A	PPB		15 Jun 2018 13:27:48	U	SMPL
J3469-02LX5 - 1		-116	-0.0482	-7470A	PPB		15 Jun 2018 13:29:55	U	SMPL
J3469-02A - 1		13574	3.7580	-7470A	PPB		15 Jun 2018 13:32:02	U	SMPL
J3469-01LX5 - 1		1616	0.4334	-7470A	PPB		15 Jun 2018 13:34:09	U	SMPL
J3469-01A - 1		19960	5.5335	-7470A	PPB		15 Jun 2018 13:36:17	U	SMPL
CCV44 - 1	CCV44	17677	4.8987	-7470A	PPB		15 Jun 2018 13:38:24	U	SMPL
CCB44 - 1	CCB44	-155	-0.0590	-7470A	PPB		15 Jun 2018 13:40:35	U	SMPL