

LB 96207


7470A

INSTRUMENT ID: CVJ

Linear

 μ Abs.:

36930

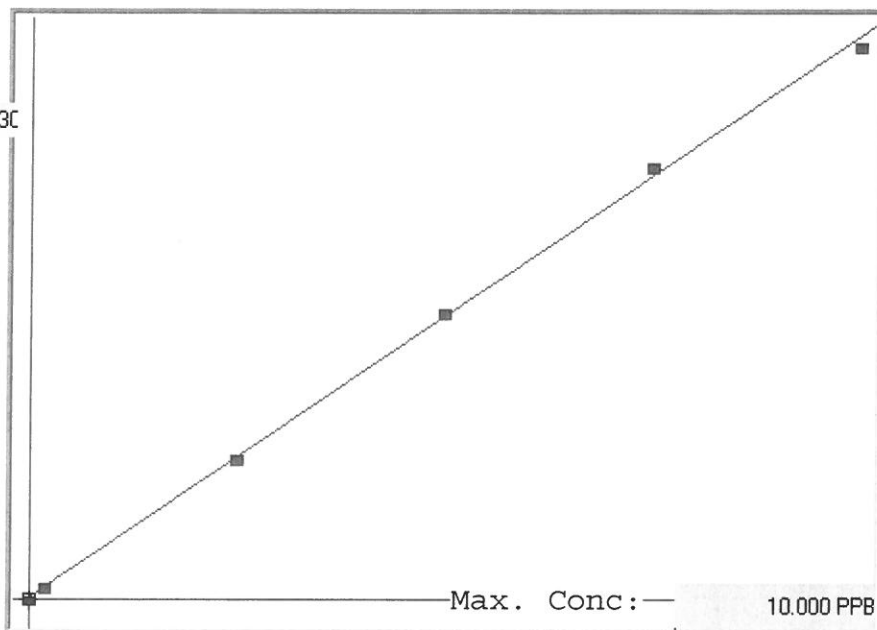

A= 0.0000e+000

B= 2.6724e-004

C= -2.8967e-002

Rho= 0.9996281

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.031	-0.031	-9	0.000	-9				
0.2	0.200	0.179	-0.021	778	0.0 %	778				
2.5	2.500	2.469	-0.031	9346	0.0 %	9346				
5.0	5.000	5.083	0.083	19128	0.0 %	19128				
7.5	7.500	7.661	0.161	28776	0.0 %	28776				
10.0	10.000	9.840	-0.160	36930	0.0 %	36930				

LB96207 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 22 Jun 2018 08:30:44

Sample ID	Extended ID	µ Abs	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-9	-	0.0000	7470A	PPB	22 Jun 2018 08:34:14	S	Std
0.2 - 1	50.2	778	-	0.2000	7470A	PPB	22 Jun 2018 08:36:22	S	Std
2.5 - 1	52.5	9346	-	2.5000	7470A	PPB	22 Jun 2018 08:38:30	S	Std
5.0 - 1	55	19128	-	5.0000	7470A	PPB	22 Jun 2018 08:40:38	S	Std
7.5 - 1	57.5	28776	-	7.5000	7470A	PPB	22 Jun 2018 08:42:46	S	Std
10.0 - 1	510	36930	-	10.0000	7470A	PPB	22 Jun 2018 08:52:29	S	Std
ICV16 - 1	ICV16	15742	4.1779	-	7470A	PPB	22 Jun 2018 08:55:06	U	SMPL
ICB16 - 1	ICB16	-105	-0.0570	-	7470A	PPB	22 Jun 2018 08:57:13	U	SMPL
CCV13 - 1	CCV13	19238	5.1121	-	7470A	PPB	22 Jun 2018 08:59:19	U	SMPL
CCB13 - 1	CCB13	-94	-0.0541	-	7470A	PPB	22 Jun 2018 09:01:25	U	SMPL
CRA - 1	CRA	807	0.1867	-	7470A	PPB	22 Jun 2018 09:03:33	U	SMPL
HighStd - 1	HighStd	36936	9.8417	-	7470A	PPB	22 Jun 2018 09:05:39	U	SMPL
ChkStd - 1	ChkStd	27003	7.1872	-	7470A	PPB	22 Jun 2018 09:07:46	U	SMPL
PB110497BL - 1	PBW	-162	-0.0723	-	7470A	PPB	22 Jun 2018 09:09:55	U	SMPL
PB110497BS - 1	LCSW	13766	3.6498	-	7470A	PPB	22 Jun 2018 09:12:04	U	SMPL
J3627-35 - 1	GROUND-WATER	2651	0.6795	-	7470A	PPB	22 Jun 2018 09:14:12	U	SMPL
J3627-35DUP - 1	GROUND-WATERDUP	2612	0.6691	-	7470A	PPB	22 Jun 2018 09:16:21	U	SMPL
J3627-35MS - 1	GROUND-WATERMS	17381	4.6159	-	7470A	PPB	22 Jun 2018 09:18:29	U	SMPL
J3627-35MSD - 1	GROUND-WATERMSD	17248	4.5803	-	7470A	PPB	22 Jun 2018 09:20:38	U	SMPL
PB110491BL - 1	PBW	-124	-0.0621	-	7470A	PPB	22 Jun 2018 09:22:45	U	SMPL
CCV14 - 1	CCV14	19091	5.0728	-	7470A	PPB	22 Jun 2018 09:24:53	U	SMPL
CCB14 - 1	CCB14	-40	-0.0397	-	7470A	PPB	22 Jun 2018 09:27:00	U	SMPL
PB110491BS - 1	LCSW	13086	3.4681	-	7470A	PPB	22 Jun 2018 09:29:07	U	SMPL
PB110491TB - 1	PB110	-251	-0.0960	-	7470A	PPB	22 Jun 2018 09:31:14	U	SMPL
J3570-10 - 1	20180373-AMENDED-COMPOSITE-CS-1A	1066	0.2559	-	7470A	PPB	22 Jun 2018 09:33:21	U	SMPL
J3570-10DUP - 1	20180373-AMENDED-COMPOSITE-CS-1ADUP	1075	0.2583	-	7470A	PPB	22 Jun 2018 09:35:28	U	SMPL
J3570-10MS - 1	20180373-AMENDED-COMPOSITE-CS-1AMS	16380	4.3484	-	7470A	PPB	22 Jun 2018 09:37:35	U	SMPL
J3570-10MSD - 1	20180373-AMENDED-COMPOSITE-CS-1AMSD	15415	4.0905	-	7470A	PPB	22 Jun 2018 09:39:43	U	SMPL
J3570-11 - 1	20180374-AMENDED-COMPOSITE-CS-1B	403	0.0787	-	7470A	PPB	22 Jun 2018 09:41:51	U	SMPL
PB110490BL - 1	PBW	-25	-0.0356	-	7470A	PPB	22 Jun 2018 09:43:59	U	SMPL
PB110490BS - 1	LCSW	13877	3.6795	-	7470A	PPB	22 Jun 2018 09:46:07	U	SMPL
PB110490TB - 1	PB110440TB	-93	-0.0538	-	7470A	PPB	22 Jun 2018 09:48:14	U	SMPL
CCV15 - 1	CCV15	19356	5.1437	-	7470A	PPB	22 Jun 2018 09:50:21	U	SMPL
CCB15 - 1	CCB15	-66	-0.0466	-	7470A	PPB	22 Jun 2018 09:52:28	U	SMPL
J3246-04 - 1	OK-01-062018	21	-0.0234	-	7470A	PPB	22 Jun 2018 09:54:36	U	SMPL
J3246-04DUP - 1	OK-01-062018DUP	2	-0.0284	-	7470A	PPB	22 Jun 2018 09:56:44	U	SMPL
J3246-04MS - 1	OK-01-062018MS	12841	3.4026	-	7470A	PPB	22 Jun 2018 09:58:50	U	SMPL
J3246-04MSD - 1	OK-01-062018MSD	13318	3.5301	-	7470A	PPB	22 Jun 2018 10:00:57	U	SMPL
J3603-02 - 1	26KV-TP-1	-94	-0.0541	-	7470A	PPB	22 Jun 2018 10:03:05	U	SMPL
J3603-04 - 1	26KV-TP-2	95	-0.0036	-	7470A	PPB	22 Jun 2018 10:05:12	U	SMPL
J3603-06 - 1	26KV-TP-3	-26	-0.0359	-	7470A	PPB	22 Jun 2018 10:07:20	U	SMPL
J3603-08 - 1	26KV-TP-4	31	-0.0207	-	7470A	PPB	22 Jun 2018 10:09:29	U	SMPL
J3603-10 - 1	26KV-TP-5	8	-0.0268	-	7470A	PPB	22 Jun 2018 10:11:37	U	SMPL
J3603-12 - 1	26KV-CSM	23	-0.0228	-	7470A	PPB	22 Jun 2018 10:13:44	U	SMPL
CCV16 - 1	CCV16	18809	4.9975	-	7470A	PPB	22 Jun 2018 10:15:51	U	SMPL
CCB16 - 1	CCB16	-119	-0.0608	-	7470A	PPB	22 Jun 2018 10:17:59	U	SMPL
J3603-14 - 1	26KV-TP-10	4	-0.0279	-	7470A	PPB	22 Jun 2018 10:20:06	U	SMPL
J3603-16 - 1	26KV-TP-9	14	-0.0252	-	7470A	PPB	22 Jun 2018 10:22:14	U	SMPL
J3603-18 - 1	26KV-TP-8	24	-0.0226	-	7470A	PPB	22 Jun 2018 10:24:21	U	SMPL
J3603-20 - 1	26KV-TP-7	42	-0.0177	-	7470A	PPB	22 Jun 2018 10:26:27	U	SMPL
J3603-22 - 1	26KV-TP-6	12	-0.0258	-	7470A	PPB	22 Jun 2018 10:28:35	U	SMPL
J3603-24 - 1	26KV-TP-11	9	-0.0266	-	7470A	PPB	22 Jun 2018 10:30:43	U	SMPL
J3611-05 - 1	N-1366-WATER	-10	-0.0316	-	7470A	PPB	22 Jun 2018 10:32:51	U	SMPL
J3622-03 - 1	275-137-282-284	35	-0.0196	-	7470A	PPB	22 Jun 2018 10:34:59	U	SMPL
J3622-07 - 1	SP-A	46	-0.0167	-	7470A	PPB	22 Jun 2018 10:37:07	U	SMPL
J3622-11 - 1	SP-B	65	-0.0116	-	7470A	PPB	22 Jun 2018 10:39:15	U	SMPL
CCV17 - 1	CCV17	18928	5.0293	-	7470A	PPB	22 Jun 2018 10:41:22	U	SMPL
CCB17 - 1	CCB17	-66	-0.0466	-	7470A	PPB	22 Jun 2018 10:43:29	U	SMPL
J3622-15 - 1	SP-C	436	0.0875	-	7470A	PPB	22 Jun 2018 10:45:37	U	SMPL
J3622-19 - 1	SP-D	386	0.0742	-	7470A	PPB	22 Jun 2018 10:47:44	U	SMPL
J3627-35LX5 - 1		741	0.1691	-	7470A	PPB	22 Jun 2018 10:49:51	U	SMPL
J3627-35A - 1		17354	4.6086	-	7470A	PPB	22 Jun 2018 10:51:58	U	SMPL
J3570-10LX5 - 1		149	0.0109	-	7470A	PPB	22 Jun 2018 10:54:05	U	SMPL
J3570-10A - 1		15580	4.1346	-	7470A	PPB	22 Jun 2018 10:56:14	U	SMPL
J3246-04LX5 - 1		-38	-0.0391	-	7470A	PPB	22 Jun 2018 10:58:21	U	SMPL
J3246-04A - 1		14147	3.7516	-	7470A	PPB	22 Jun 2018 11:00:30	U	SMPL
CCV18 - 1	CCV18	19090	5.0726	-	7470A	PPB	22 Jun 2018 11:02:38	U	SMPL
CCB18 - 1	CCB18	-100	-0.0557	-	7470A	PPB	22 Jun 2018 11:04:45	U	SMPL