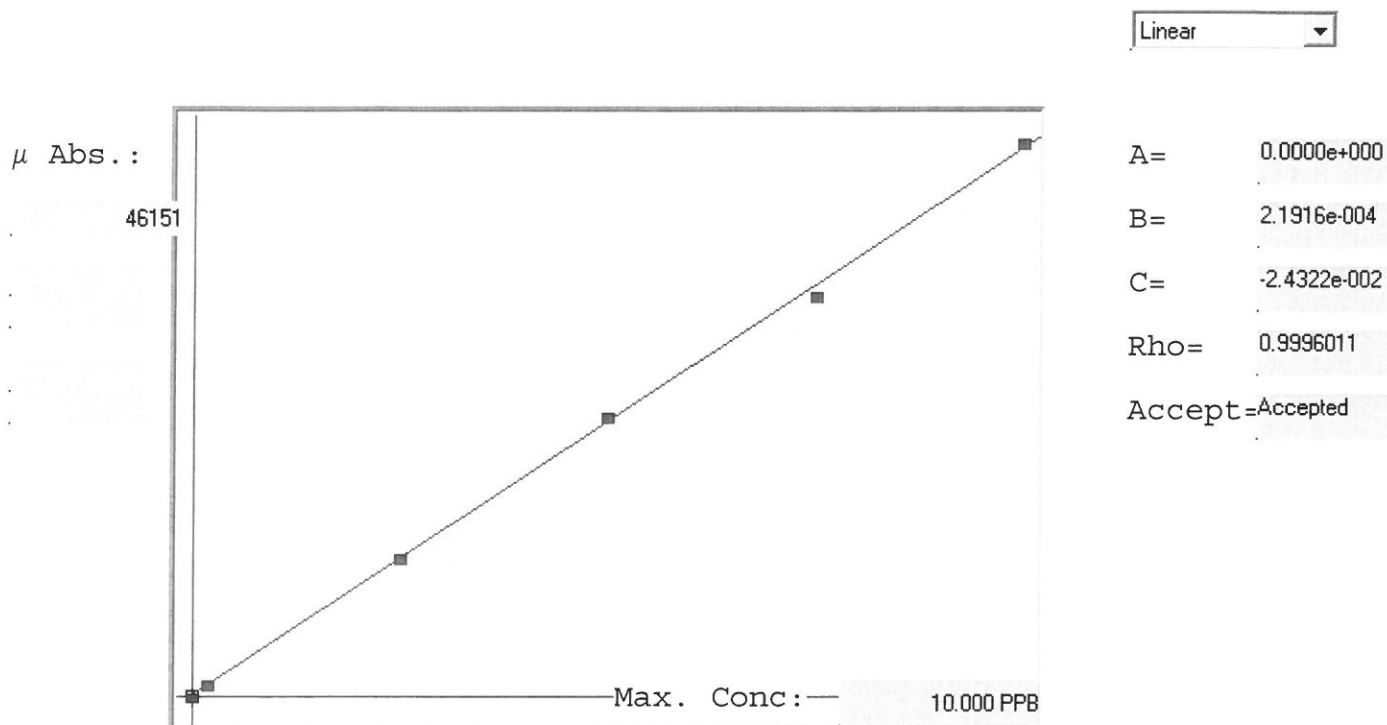


7471B

LB 96225
INSTRUMENT ID: CV1

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.013	-0.013	50	0.000	50				
0.2	0.200	0.207	0.007	1054	0.0 %	1054				
2.5	2.500	2.511	0.011	11569	0.0 %	11569				
5.0	5.000	5.114	0.114	23448	0.0 %	23448				
7.5	7.500	7.291	-0.209	33380	0.0 %	33380				
10.0	10.000	10.090	0.090	46151	0.0 %	46151				

LB96225 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 22 Jun 2018 15:19:26

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	50	-	0.0000	7471B	PPB	22 Jun 2018 15:21:56	S	Std
0.2 - 1	50.2	1054	-	0.2000	7471B	PPB	22 Jun 2018 15:24:14	S	Std
2.5 - 1	52.5	11569	-	2.5000	7471B	PPB	22 Jun 2018 15:26:32	S	Std
5.0 - 1	55	23448	-	5.0000	7471B	PPB	22 Jun 2018 15:28:49	S	Std
7.5 - 1	57.5	33380	-	7.5000	7471B	PPB	22 Jun 2018 15:31:06	S	Std
10.0 - 1	510	46151	-	10.0000	7471B	PPB	22 Jun 2018 15:33:24	S	Std
ICV17 - 1	ICV17	18487	4.0272	-	7471B	PPB	22 Jun 2018 15:36:06	U	SMPL
ICB17 - 1	ICB17	-124	-0.0515	-	7471B	PPB	22 Jun 2018 15:38:22	U	SMPL
CCV21 - 1	CCV21	23402	5.1044	-	7471B	PPB	22 Jun 2018 15:40:37	U	SMPL
CCB21 - 1	CCB21	-121	-0.0508	-	7471B	PPB	22 Jun 2018 15:42:53	U	SMPL
CRA - 1	CRA	1056	0.2071	-	7471B	PPB	22 Jun 2018 15:45:09	U	SMPL
HighStd - 1	HighStd	46109	10.0808	-	7471B	PPB	22 Jun 2018 15:47:24	U	SMPL
ChkStd - 1	ChkStd	32366	7.0689	-	7471B	PPB	22 Jun 2018 15:49:40	U	SMPL
PB110498BL - 1	PBS	-167	-0.0609	-	7471B	PPB	22 Jun 2018 15:51:58	U	SMPL
PB110498BS - 1	LCSS	16976	3.6961	-	7471B	PPB	22 Jun 2018 15:54:16	U	SMPL
J3252-03 - 1	TR-05-062118	984	0.1913	-	7471B	PPB	22 Jun 2018 15:56:33	U	SMPL
J3252-03DUP - 1	TR-05-062118DUP	825	0.1565	-	7471B	PPB	22 Jun 2018 16:01:49	U	SMPL
J3252-03MS - 1	TR-05-062118MS	18254	3.9762	-	7471B	PPB	22 Jun 2018 16:04:06	U	SMPL
J3252-03MSD - 1	TR-05-062118MSD	18140	3.9512	-	7471B	PPB	22 Jun 2018 16:06:24	U	SMPL
J3638-01 - 1	P-1	5545	1.1909	-	7471B	PPB	22 Jun 2018 16:08:40	U	SMPL
CCV22 - 1	CCV22	23413	5.1068	-	7471B	PPB	22 Jun 2018 16:10:56	U	SMPL
CCB22 - 1	CCB22	-111	-0.0486	-	7471B	PPB	22 Jun 2018 16:13:12	U	SMPL
J3638-02 - 1	P-2	5145	1.1032	-	7471B	PPB	22 Jun 2018 16:15:28	U	SMPL
J3638-03 - 1	P-3	4624	0.9891	-	7471B	PPB	22 Jun 2018 16:17:44	U	SMPL
J3642-01 - 1	TEST-PIT-1	10820	2.3470	-	7471B	PPB	22 Jun 2018 16:20:00	U	SMPL
J3642-05 - 1	TEST-PIT-2	29061	6.3446	-	7471B	PPB	22 Jun 2018 16:22:17	U	SMPL
J3665-01 - 1	EPE-105-4(90-92)	122	0.0024	-	7471B	PPB	22 Jun 2018 16:24:34	U	SMPL
J3665-02 - 1	EPE-105-4(95-97)	106	-0.0011	-	7471B	PPB	22 Jun 2018 16:26:52	U	SMPL
J3665-03 - 1	EPE-105-4(110-112)	195	0.0184	-	7471B	PPB	22 Jun 2018 16:29:10	U	SMPL
J3252-03LX5 - 1		202	0.0199	-	7471B	PPB	22 Jun 2018 16:35:46	U	SMPL
J3252-03A - 1		18322	3.9911	-	7471B	PPB	22 Jun 2018 16:38:04	U	SMPL
CCV23 - 1	CCV23	23212	5.0627	-	7471B	PPB	22 Jun 2018 16:40:20	U	SMPL
CCB23 - 1	CCB23	-111	-0.0486	-	7471B	PPB	22 Jun 2018 16:42:36	U	SMPL