


7470A

L396399
INSTRUMENT ID: EV1

Linear

 μ Abs.:

37213

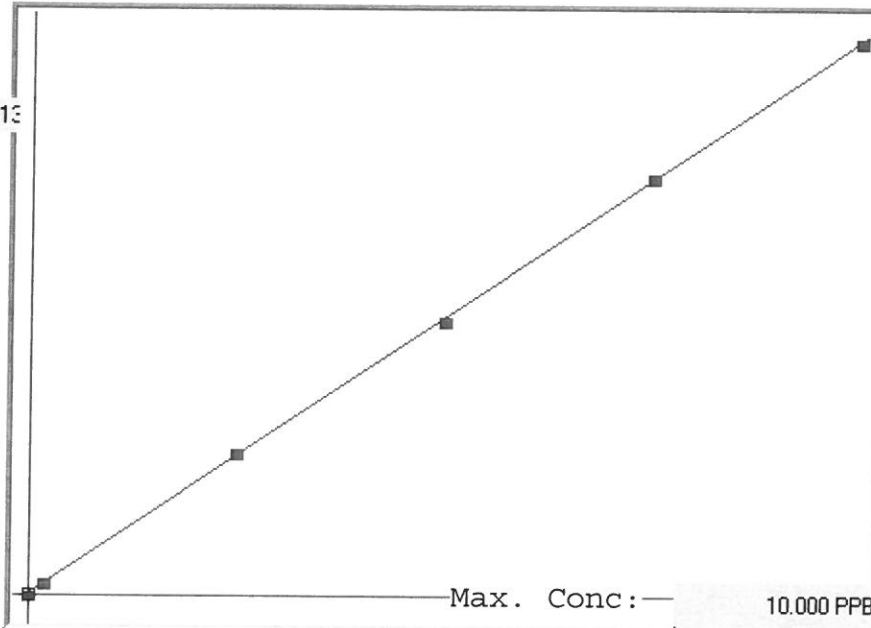

A= 0.0000e+000

B= 2.6886e-004

C= -2.9208e-002

Rho= 0.9999304

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.019	-0.019	37	0.000	37				
0.2	0.200	0.188	-0.012	807	0.0 %	807				
2.5	2.500	2.567	0.067	9655	0.0 %	9655				
5.0	5.000	4.941	-0.059	18485	0.0 %	18485				
7.5	7.500	7.548	0.048	28183	0.0 %	28183				
10.0	10.000	9.976	-0.024	37213	0.0 %	37213				

LB96399 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 03 Jul 2018 09:33:02

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	S0	37	-	0.00007470A	PPB		03 Jul 2018 09:57:21	S	Std
0.2 - 1	S02	807	-	0.20007470A	PPB		03 Jul 2018 09:59:31	S	Std
2.5 - 1	S2.5	9655	-	2.50007470A	PPB		03 Jul 2018 10:01:39	S	Std
5.0 - 1	S5	18485	-	5.00007470A	PPB		03 Jul 2018 10:03:47	S	Std
7.5 - 1	S7.5	28183	-	7.50007470A	PPB		03 Jul 2018 10:05:55	S	Std
10.0 - 1	S10	37213	-	10.00007470A	PPB		03 Jul 2018 10:08:02	S	Std
ICV32 - 1	ICV32	13901	3.7083	-7470A	PPB		03 Jul 2018 10:10:47	U	SMPL
ICB32 - 1	ICB32	-137	-0.0660	-7470A	PPB		03 Jul 2018 10:12:53	U	SMPL
CCV95 - 1	CCV95	18793	5.0235	-7470A	PPB		03 Jul 2018 10:15:01	U	SMPL
CCB95 - 1	CCB95	-164	-0.0733	-7470A	PPB		03 Jul 2018 10:17:07	U	SMPL
CRA - 1	CRA	819	0.1910	-7470A	PPB		03 Jul 2018 10:19:14	U	SMPL
HighStd - 1	HighStd	37736	10.1166	-7470A	PPB		03 Jul 2018 10:21:21	U	SMPL
ChkStd - 1	ChkStd	26146	7.0005	-7470A	PPB		03 Jul 2018 10:23:28	U	SMPL
PB110777BL - 1	PBW	-145	-0.0682	-7470A	PPB		03 Jul 2018 10:25:37	U	SMPL
PB110777BS - 1	LCSW	13542	3.6117	-7470A	PPB		03 Jul 2018 10:27:46	U	SMPL
PB110777TB - 1	PB110743TB	-72	-0.0486	-7470A	PPB		03 Jul 2018 10:29:54	U	SMPL
J3243-06 - 1	NB-08-062918	-23	-0.0354	-7470A	PPB		03 Jul 2018 10:32:02	U	SMPL
J3243-06DUP - 1	NB-08-062918DUP	9	-0.0268	-7470A	PPB		03 Jul 2018 10:34:10	U	SMPL
J3243-06MS - 1	NB-08-062918MS	13158	3.5085	-7470A	PPB		03 Jul 2018 10:36:19	U	SMPL
J3243-06MSD - 1	NB-08-062918MSD	13838	3.6913	-7470A	PPB		03 Jul 2018 10:38:26	U	SMPL
CCV96 - 1	CCV96	18785	5.0214	-7470A	PPB		03 Jul 2018 10:40:32	U	SMPL
CCB96 - 1	CCB96	-107	-0.0580	-7470A	PPB		03 Jul 2018 10:42:39	U	SMPL
J3245-18 - 1	CL-01-062918-A	-7	-0.0311	-7470A	PPB		03 Jul 2018 10:44:46	U	SMPL
J3245-20 - 1	CL-01-062918-B	8	-0.0271	-7470A	PPB		03 Jul 2018 10:46:52	U	SMPL
J3245-22 - 1	CL-01-062918-C	-2	-0.0297	-7470A	PPB		03 Jul 2018 10:48:59	U	SMPL
J3245-24 - 1	CL-01-062918-D	-13	-0.0327	-7470A	PPB		03 Jul 2018 10:51:06	U	SMPL
J3248-08 - 1	EO-03-062818-A	-49	-0.0424	-7470A	PPB		03 Jul 2018 10:53:13	U	SMPL
J3248-10 - 1	EO-03-062818-B	18	-0.0244	-7470A	PPB		03 Jul 2018 10:55:21	U	SMPL
J3248-12 - 1	EO-03-062818-C	16	-0.0249	-7470A	PPB		03 Jul 2018 10:57:29	U	SMPL
J3252-06 - 1	TR-04-062918	45	-0.0171	-7470A	PPB		03 Jul 2018 10:59:38	U	SMPL
J3771-02 - 1	Reactor-Pad	46	-0.0168	-7470A	PPB		03 Jul 2018 11:01:46	U	SMPL
J3790-01 - 1	ZER-WC-S-01-0-72	90	-0.0050	-7470A	PPB		03 Jul 2018 11:03:53	U	SMPL
CCV97 - 1	CCV97	18635	4.9810	-7470A	PPB		03 Jul 2018 11:06:00	U	SMPL
CCB97 - 1	CCB97	-104	-0.0572	-7470A	PPB		03 Jul 2018 11:08:07	U	SMPL
J3796-02 - 1	JC-SOIL	51	-0.0155	-7470A	PPB		03 Jul 2018 11:10:15	U	SMPL
PB110778BL - 1	PBW	73	-0.0096	-7470A	PPB		03 Jul 2018 11:12:22	U	SMPL
PB110778BS - 1	LCSW	13076	3.4864	-7470A	PPB		03 Jul 2018 11:14:29	U	SMPL
PB110778TB - 1	PB110752TB	-98	-0.0556	-7470A	PPB		03 Jul 2018 11:16:36	U	SMPL
J3755-02 - 1	PS-BASELINEWATER	26	-0.0222	-7470A	PPB		03 Jul 2018 11:18:43	U	SMPL
J3755-02DUP - 1	PS-BASELINEWATERDUP	3	-0.0284	-7470A	PPB		03 Jul 2018 11:20:51	U	SMPL
J3755-02MS - 1	PS-BASELINEWATERMS	13833	3.6900	-7470A	PPB		03 Jul 2018 11:22:59	U	SMPL
J3755-02MSD - 1	PS-BASELINEWATERMSD	13852	3.6951	-7470A	PPB		03 Jul 2018 11:25:07	U	SMPL
J3798-02 - 1	DRUM-1-6	-25	-0.0359	-7470A	PPB		03 Jul 2018 11:27:15	U	SMPL
J3798-05 - 1	DRUM-7-12	108	-0.0002	-7470A	PPB		03 Jul 2018 11:29:22	U	SMPL
CCV98 - 1	CCV98	18687	4.9950	-7470A	PPB		03 Jul 2018 11:31:29	U	SMPL
CCB98 - 1	CCB98	-134	-0.0652	-7470A	PPB		03 Jul 2018 11:33:36	U	SMPL
J3798-08 - 1	DRUM-13	156	0.0127	-7470A	PPB		03 Jul 2018 11:35:44	U	SMPL
PB110809BL - 1	PBW	203	0.0254	-7470A	PPB		03 Jul 2018 11:37:51	U	SMPL
PB110809BS - 1	LCSW	13373	3.5663	-7470A	PPB		03 Jul 2018 11:39:57	U	SMPL
J3790-02 - 1	ZER-WC-L-01	475	0.0985	-7470A	PPB		03 Jul 2018 11:42:05	U	SMPL
J3798-01 - 1	DRUM-1-6	239	0.0350	-7470A	PPB		03 Jul 2018 11:44:12	U	SMPL
J3798-01DUP - 1	DRUM-1-6DUP	190	0.0219	-7470A	PPB		03 Jul 2018 11:46:20	U	SMPL
J3798-01MS - 1	DRUM-1-6MS	15666	4.1828	-7470A	PPB		03 Jul 2018 11:51:00	U	SMPL
J3798-01MSD - 1	DRUM-1-6MSD	16632	4.4425	-7470A	PPB		03 Jul 2018 11:53:07	U	SMPL
J3798-04 - 1	DRUM-7-12	-197	-0.0822	-7470A	PPB		03 Jul 2018 11:55:18	U	SMPL
J3798-07 - 1	DRUM-13	5929	1.5649	-7470A	PPB		03 Jul 2018 11:57:26	U	SMPL
CCV99 - 1	CCV99	18297	4.8902	-7470A	PPB		03 Jul 2018 11:59:33	U	SMPL
CCB99 - 1	CCB99	-149	-0.0693	-7470A	PPB		03 Jul 2018 12:01:41	U	SMPL
J3743-02 - 1	GMW-5	-105	-0.0574	-7470A	PPB		03 Jul 2018 12:03:48	U	SMPL
J3243-06LX5 - 1		2	-0.0287	-7470A	PPB		03 Jul 2018 12:05:55	U	SMPL
J3243-06A - 1		14500	3.8693	-7470A	PPB		03 Jul 2018 12:08:03	U	SMPL
J3755-02LX5 - 1		-76	-0.0496	-7470A	PPB		03 Jul 2018 12:10:10	U	SMPL
J3755-02A - 1		14481	3.8642	-7470A	PPB		03 Jul 2018 12:12:17	U	SMPL
J3798-01LX5 - 1		-71	-0.0483	-7470A	PPB		03 Jul 2018 12:14:25	U	SMPL
J3798-01A - 1		16387	4.3766	-7470A	PPB		03 Jul 2018 12:16:33	U	SMPL
CCV01 - 1	CCV01	18264	4.8813	-7470A	PPB		03 Jul 2018 12:18:41	U	SMPL
CCB01 - 1	CCB01	-131	-0.0644	-7470A	PPB		03 Jul 2018 12:20:50	U	SMPL