


7470A

LB96436
INSTRUMENT ID: CV2

Linear

 μ Abs.:

42059

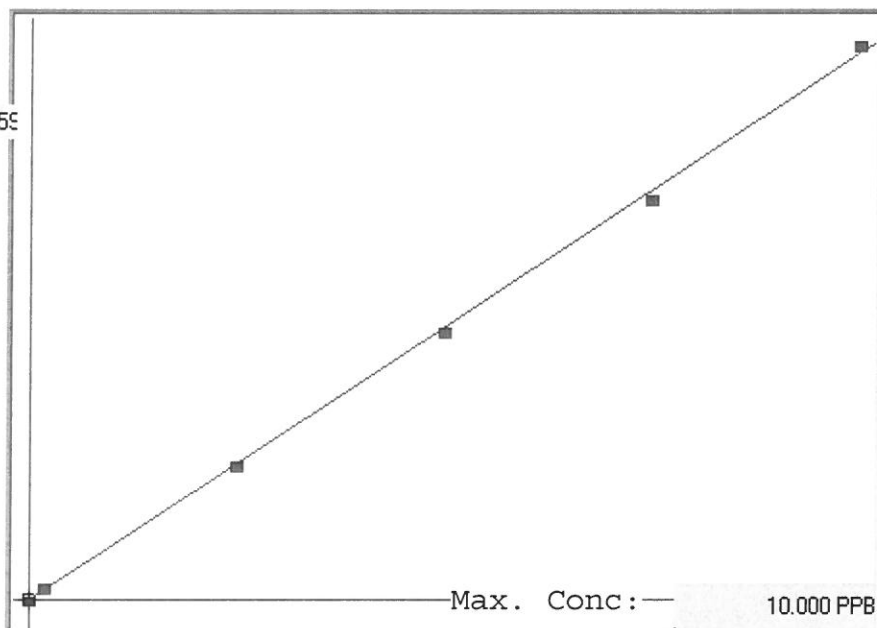

A= 0.0000e+000

B= 2.4064e-004

C= 1.7741e-002

Rho= 0.9996991

Accept= Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.040	0.040	91	0.000	91				
0.2	0.200	0.232	0.032	892	0.0 %	892				
2.5	2.500	2.502	0.002	10323	0.0 %	10323				
5.0	5.000	4.941	-0.059	20460	0.0 %	20460				
7.5	7.500	7.346	-0.154	30452	0.0 %	30452				
10.0	10.000	10.139	0.139	42059	0.0 %	42059				

LB96436 INSTRUMENT ID : ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 05 Jul 2018 11:03:13

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	91	-	0.00007470A	PPB		05 Jul 2018 11:04:52	S	Std
0.2 - 1	50.2	892	-	0.20007470A	PPB		05 Jul 2018 11:07:00	S	Std
2.5 - 1	52.5	10323	-	2.50007470A	PPB		05 Jul 2018 11:09:08	S	Std
5.0 - 1	55	20460	-	5.00007470A	PPB		05 Jul 2018 11:11:17	S	Std
7.5 - 1	57.5	30452	-	7.50007470A	PPB		05 Jul 2018 11:13:24	S	Std
10.0 - 1	510	42059	-	10.00007470A	PPB		05 Jul 2018 11:15:32	S	Std
ICV36 - 1	ICV36	15538	3.7569	-7470A	PPB		05 Jul 2018 11:18:14	U	SMPL
ICB36 - 1	ICB36	-91	-0.0042	-7470A	PPB		05 Jul 2018 11:20:20	U	SMPL
CCV13 - 1	CCV13	20494	4.9495	-7470A	PPB		05 Jul 2018 11:22:26	U	SMPL
CCB13 - 1	CCB13	-74	-0.0001	-7470A	PPB		05 Jul 2018 11:24:33	U	SMPL
CRA - 1	CRA	903	0.2350	-7470A	PPB		05 Jul 2018 11:26:40	U	SMPL
HighStd - 1	HighStd	41609	10.0307	-7470A	PPB		05 Jul 2018 11:28:47	U	SMPL
ChkStd - 1	ChkStd	28748	6.9358	-7470A	PPB		05 Jul 2018 11:30:53	U	SMPL
PB110821BL - 1	PBW	-128	-0.0131	-7470A	PPB		05 Jul 2018 11:33:02	U	SMPL
PB110821BS - 1	LCSW	14987	3.6243	-7470A	PPB		05 Jul 2018 11:35:11	U	SMPL
PB110821TB - 1	PB110795TB	-74	-0.0001	-7470A	PPB		05 Jul 2018 11:37:18	U	SMPL
J3812-01 - 1	DPC-81753-FB-05	22	0.0230	-7470A	PPB		05 Jul 2018 11:39:26	U	SMPL
J3812-02 - 1	DPC-81753-FB-06	27	0.0242	-7470A	PPB		05 Jul 2018 11:41:35	U	SMPL
J3812-03 - 1	DPC-81753-FB-07	28	0.0245	-7470A	PPB		05 Jul 2018 11:43:43	U	SMPL
J3812-04 - 1	DPC-81753-FB-04	235	0.0743	-7470A	PPB		05 Jul 2018 11:45:50	U	SMPL
CCV14 - 1	CCV14	20445	4.9377	-7470A	PPB		05 Jul 2018 11:47:56	U	SMPL
CCB14 - 1	CCB14	-61	0.0031	-7470A	PPB		05 Jul 2018 11:50:02	U	SMPL
J3812-05 - 1	DPC-81753-FB-09	255	0.0791	-7470A	PPB		05 Jul 2018 11:52:09	U	SMPL
J3812-06 - 1	DPC-81753-FB-03	287	0.0868	-7470A	PPB		05 Jul 2018 11:54:16	U	SMPL
J3814-03 - 1	8782-AA	363	0.1051	-7470A	PPB		05 Jul 2018 11:56:23	U	SMPL
J3815-03 - 1	964	417	0.1181	-7470A	PPB		05 Jul 2018 11:58:29	U	SMPL
J3816-01 - 1	159-CONC-FLOOR	936	0.2430	-7470A	PPB		05 Jul 2018 12:00:37	U	SMPL
J3816-02 - 1	159-WHITE-BLOCK	101719	24.4957	-7470A	PPB		05 Jul 2018 12:02:44	U	SMPL
J3816-03 - 1	159-WHITE-BRICK	46089	11.1087	-7470A	PPB		05 Jul 2018 12:04:53	U	SMPL
J3816-04 - 1	159-WHITE-BLUE-BRICK	548	0.1496	-7470A	PPB		05 Jul 2018 12:07:04	U	SMPL
J3816-06 - 1	161-TAN-BRICK	1046	0.2695	-7470A	PPB		05 Jul 2018 12:09:15	U	SMPL
J3816-09 - 1	161-CONC-GREEN-WALL	85	0.0382	-7470A	PPB		05 Jul 2018 12:11:21	U	SMPL
CCV15 - 1	CCV15	20616	4.9788	-7470A	PPB		05 Jul 2018 12:13:28	U	SMPL
CCB15 - 1	CCB15	-83	-0.0022	-7470A	PPB		05 Jul 2018 12:15:35	U	SMPL
J3818-03 - 1	5002	301	0.0902	-7470A	PPB		05 Jul 2018 12:17:43	U	SMPL
J3826-02 - 1	OK-03-070218	2828	0.6983	-7470A	PPB		05 Jul 2018 12:19:50	U	SMPL
J3840-04 - 1	TP-6-S	29	0.0247	-7470A	PPB		05 Jul 2018 12:21:56	U	SMPL
J3840-09 - 1	TP-6-D	35	0.0262	-7470A	PPB		05 Jul 2018 12:24:03	U	SMPL
J3840-13 - 1	TP-4-S	10	0.0201	-7470A	PPB		05 Jul 2018 12:26:11	U	SMPL
J3840-18 - 1	TP-4-D	49	0.0295	-7470A	PPB		05 Jul 2018 12:28:19	U	SMPL
J3840-18DUP - 1	TP-4-DDUP	78	0.0365	-7470A	PPB		05 Jul 2018 12:30:27	U	SMPL
J3840-18MS - 1	TP-4-DMS	14542	3.5172	-7470A	PPB		05 Jul 2018 12:32:35	U	SMPL
J3840-18MSD - 1	TP-4-DMSD	15289	3.6969	-7470A	PPB		05 Jul 2018 12:34:43	U	SMPL
CCV16 - 1	CCV16	19681	4.7538	-7470A	PPB		05 Jul 2018 12:36:50	U	SMPL
CCB16 - 1	CCB16	-64	0.0023	-7470A	PPB		05 Jul 2018 12:38:58	U	SMPL
J3840-18LX5 - 1		39	0.0271	-7470A	PPB		05 Jul 2018 12:41:05	U	SMPL
J3840-18A - 1		14777	3.5737	-7470A	PPB		05 Jul 2018 12:43:12	U	SMPL
J3816-02DLX5 - 1		19401	4.6865	-7470A	PPB		05 Jul 2018 12:45:20	U	SMPL
J3816-03DLX2 - 1		22716	5.4842	-7470A	PPB		05 Jul 2018 12:47:26	U	SMPL
CCV17 - 1	CCV17	20593	4.9733	-7470A	PPB		05 Jul 2018 12:49:34	U	SMPL
CCB17 - 1	CCB17	-110	-0.0087	-7470A	PPB		05 Jul 2018 12:51:42	U	SMPL