


7470A

LB 96444
INSTRUMENT ID: CV1

Linear

 μ Abs.:

37673

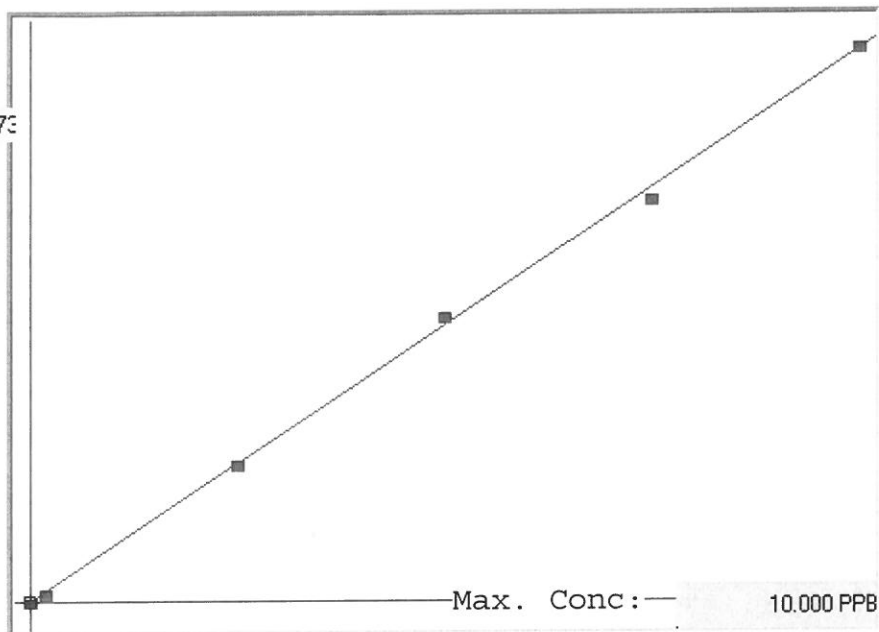

A= 0.0000e+000

B= 2.6688e-004

C= 4.1840e-003

Rho= 0.9995462

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.006	-0.006	-37	0.000	-37				
0.2	0.200	0.174	-0.026	635	0.0 %	635				
2.5	2.500	2.506	0.006	9374	0.0 %	9374				
5.0	5.000	5.170	0.170	19357	0.0 %	19357				
7.5	7.500	7.298	-0.202	27328	0.0 %	27328				
10.0	10.000	10.058	0.058	37673	0.0 %	37673				

LB96444 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 05 Jul 2018 14:54:23

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-37	-	0.00007470A	PPB		05 Jul 2018 14:56:52	S	Std
0.2 - 1	50.2	635	-	0.20007470A	PPB		05 Jul 2018 14:59:00	S	Std
2.5 - 1	52.5	9374	-	2.50007470A	PPB		05 Jul 2018 15:01:08	S	Std
5.0 - 1	55	19357	-	5.00007470A	PPB		05 Jul 2018 15:03:16	S	Std
7.5 - 1	57.5	27328	-	7.50007470A	PPB		05 Jul 2018 15:05:24	S	Std
10.0 - 1	510	37673	-	10.00007470A	PPB		05 Jul 2018 15:09:59	S	Std
ICV37 - 1	ICV37	14372	3.8398	-7470A	PPB		05 Jul 2018 15:12:32	U	SMPL
ICB37 - 1	ICB37	-137	-0.0324	-7470A	PPB		05 Jul 2018 15:14:38	U	SMPL
CCV18 - 1	CCV18	19320	5.1603	-7470A	PPB		05 Jul 2018 15:19:22	U	SMPL
CCB18 - 1	CCB18	-173	-0.0420	-7470A	PPB		05 Jul 2018 15:21:28	U	SMPL
CRA - 1	CRA	642	0.1755	-7470A	PPB		05 Jul 2018 15:23:35	U	SMPL
HighStd - 1	HighStd	37304	9.9599	-7470A	PPB		05 Jul 2018 15:25:41	U	SMPL
ChkStd - 1	ChkStd	27056	7.2249	-7470A	PPB		05 Jul 2018 15:27:48	U	SMPL
PB110843BL - 1	PBW	-259	-0.0649	-7470A	PPB		05 Jul 2018 15:29:57	U	SMPL
PB110843BS - 1	LCSW	13895	3.7125	-7470A	PPB		05 Jul 2018 15:32:06	U	SMPL
PB110843TB - 1	PB110827TB	-164	-0.0396	-7470A	PPB		05 Jul 2018 15:34:13	U	SMPL
J3816-05 - 1	159-BLUE-BLOCK	-34	-0.0049	-7470A	PPB		05 Jul 2018 15:36:21	U	SMPL
J3820-02 - 1	BU-03-070318	-82	-0.0177	-7470A	PPB		05 Jul 2018 15:38:29	U	SMPL
J3843-02 - 1	CHRT20426	-23	-0.0020	-7470A	PPB		05 Jul 2018 15:40:38	U	SMPL
J3852-10 - 1	HC-SOIL-1	-49	-0.0089	-7470A	PPB		05 Jul 2018 15:42:45	U	SMPL
CCV19 - 1	CCV19	18645	4.9802	-7470A	PPB		05 Jul 2018 15:49:35	U	SMPL
CCB19 - 1	CCB19	-176	-0.0428	-7470A	PPB		05 Jul 2018 15:51:41	U	SMPL
J3852-20 - 1	HC-SOIL-2	-65	-0.0132	-7470A	PPB		05 Jul 2018 15:53:48	U	SMPL
J3852-30 - 1	HC-CON	-75	-0.0158	-7470A	PPB		05 Jul 2018 15:55:55	U	SMPL
J3854-02 - 1	S4	-65	-0.0132	-7470A	PPB		05 Jul 2018 15:58:01	U	SMPL
J3854-04 - 1	S5	-69	-0.0142	-7470A	PPB		05 Jul 2018 16:00:08	U	SMPL
J3866-02 - 1	AG-OILY-DEBRIS	-76	-0.0161	-7470A	PPB		05 Jul 2018 16:02:16	U	SMPL
J3868-04 - 1	TP-7-S	-63	-0.0126	-7470A	PPB		05 Jul 2018 16:04:23	U	SMPL
J3868-08 - 1	TP-7-D	-48	-0.0086	-7470A	PPB		05 Jul 2018 16:06:31	U	SMPL
J3868-12 - 1	TP-TP-5-S	-48	-0.0086	-7470A	PPB		05 Jul 2018 16:08:39	U	SMPL
J3868-12DUP - 1	TP-TP-5-SDUP	-46	-0.0081	-7470A	PPB		05 Jul 2018 16:10:48	U	SMPL
J3868-12MS - 1	TP-TP-5-SMS	14116	3.7715	-7470A	PPB		05 Jul 2018 16:12:54	U	SMPL
CCV20 - 1	CCV20	18837	5.0314	-7470A	PPB		05 Jul 2018 16:15:01	U	SMPL
CCB20 - 1	CCB20	-152	-0.0364	-7470A	PPB		05 Jul 2018 16:17:08	U	SMPL
J3868-12MSD - 1	TP-TP-5-SMSD	15093	4.0322	-7470A	PPB		05 Jul 2018 16:19:16	U	SMPL
PB110845BL - 1	PBW	-117	-0.0270	-7470A	PPB		05 Jul 2018 16:21:23	U	SMPL
PB110845BS - 1	LCSW	13644	3.6455	-7470A	PPB		05 Jul 2018 16:23:29	U	SMPL
PB110845TB - 1	PB110852TB	-74	-0.0156	-7470A	PPB		05 Jul 2018 16:25:36	U	SMPL
J3866-04 - 1	AG-OILY-WATER	-1	0.0039	-7470A	PPB		05 Jul 2018 16:27:44	U	SMPL
J3866-04DUP - 1	AG-OILY-WATERDUP	1	0.0045	-7470A	PPB		05 Jul 2018 16:29:51	U	SMPL
J3866-04MS - 1	AG-OILY-WATERMS	14597	3.8998	-7470A	PPB		05 Jul 2018 16:31:59	U	SMPL
J3866-04MSD - 1	AG-OILY-WATERMSD	13916	3.7181	-7470A	PPB		05 Jul 2018 16:34:08	U	SMPL
PB110846BL - 1	PBW	-139	-0.0329	-7470A	PPB		05 Jul 2018 16:36:17	U	SMPL
PB110846BS - 1	LCSW	14135	3.7765	-7470A	PPB		05 Jul 2018 16:38:24	U	SMPL
CCV21 - 1	CCV21	19067	5.0928	-7470A	PPB		05 Jul 2018 16:43:06	U	SMPL
CCB21 - 1	CCB21	-173	-0.0420	-7470A	PPB		05 Jul 2018 16:45:13	U	SMPL
J3866-03 - 1	AG-OILY-WATER	146	0.0431	-7470A	PPB		05 Jul 2018 16:47:21	U	SMPL
J3869-01 - 1	TW-3	7552	2.0197	-7470A	PPB		05 Jul 2018 16:49:28	U	SMPL
J3869-02 - 1	TW-1	2059	0.5537	-7470A	PPB		05 Jul 2018 16:51:35	U	SMPL
J3869-03 - 1	TW-2	1507	0.4064	-7470A	PPB		05 Jul 2018 16:53:43	U	SMPL
J3869-03DUP - 1	TW-2DUP	1513	0.4080	-7470A	PPB		05 Jul 2018 16:55:51	U	SMPL
J3869-03MS - 1	TW-2MS	18192	4.8593	-7470A	PPB		05 Jul 2018 16:57:58	U	SMPL
J3869-03MSD - 1	TW-2MSD	17828	4.7621	-7470A	PPB		05 Jul 2018 17:00:07	U	SMPL
CCV22 - 1	CCV22	18725	5.0015	-7470A	PPB		05 Jul 2018 17:02:15	U	SMPL
CCB22 - 1	CCB22	-157	-0.0377	-7470A	PPB		05 Jul 2018 17:04:23	U	SMPL
J3868-12LX5 - 1		-64	-0.0129	-7470A	PPB		05 Jul 2018 17:06:31	U	SMPL
J3868-12A - 1		14238	3.8040	-7470A	PPB		05 Jul 2018 17:08:38	U	SMPL
J3866-04LX5 - 1		-109	-0.0249	-7470A	PPB		05 Jul 2018 17:10:45	U	SMPL
J3866-04A - 1		13952	3.7277	-7470A	PPB		05 Jul 2018 17:12:52	U	SMPL
J3869-03LX5 - 1		464	0.1280	-7470A	PPB		05 Jul 2018 17:14:59	U	SMPL
J3869-03A - 1		19324	5.1614	-7470A	PPB		05 Jul 2018 17:17:06	U	SMPL
CCV23 - 1	CCV23	18656	4.9831	-7470A	PPB		05 Jul 2018 17:19:13	U	SMPL
CCB23 - 1	CCB23	-159	-0.0383	-7470A	PPB		05 Jul 2018 17:21:22	U	SMPL