

LB 96553


7470A

INSTRUMENT ID: CV2

Linear

μ Abs.:

37809

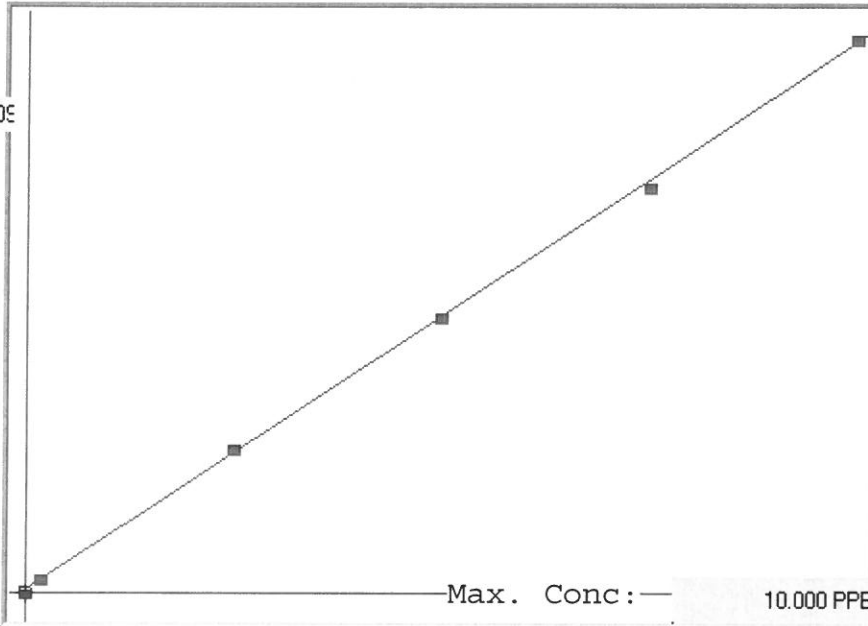

A= 0.0000e+000

B= 2.6740e-004

C= -5.5479e-002

Rho= 0.9998460

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.055	-0.055	3	0.000	3				
0.2	0.200	0.219	0.019	1027	0.0 %	1027				
2.5	2.500	2.583	0.083	9866	0.0 %	9866				
5.0	5.000	5.007	0.007	18934	0.0 %	18934				
7.5	7.500	7.391	-0.109	27847	0.0 %	27847				
10.0	10.000	10.055	0.055	37809	0.0 %	37809				

LB96553 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 11 Jul 2018 10:03:41

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	3	-	0.00007470A	PPB		11 Jul 2018 10:09:55	S	Std
0.2 - 1	50.2	1027	-	0.20007470A	PPB		11 Jul 2018 10:12:04	S	Std
2.5 - 1	52.5	9866	-	2.50007470A	PPB		11 Jul 2018 10:14:12	S	Std
5.0 - 1	55	18934	-	5.00007470A	PPB		11 Jul 2018 10:16:20	S	Std
7.5 - 1	57.5	27847	-	7.50007470A	PPB		11 Jul 2018 10:18:28	S	Std
10.0 - 1	510	37809	-	10.00007470A	PPB		11 Jul 2018 10:20:36	S	Std
ICV43 - 1	ICV43	14425	3.8018	-7470A	PPB		11 Jul 2018 10:23:13	U	SMPL
ICB43 - 1	ICB43	381	0.0464	-7470A	PPB		11 Jul 2018 10:25:19	U	SMPL
CCV47 - 1	CCV47	18943	5.0099	-7470A	PPB		11 Jul 2018 10:27:26	U	SMPL
CCB47 - 1	CCB47	132	-0.0202	-7470A	PPB		11 Jul 2018 10:29:32	U	SMPL
CRA - 1	CRA	1003	0.2127	-7470A	PPB		11 Jul 2018 10:31:40	U	SMPL
HighStd - 1	HighStd	37889	10.0760	-7470A	PPB		11 Jul 2018 10:33:46	U	SMPL
ChkStd - 1	ChkStd	25970	6.8889	-7470A	PPB		11 Jul 2018 10:35:53	U	SMPL
PB110979BL - 1	PBW	58	-0.0400	-7470A	PPB		11 Jul 2018 10:38:02	U	SMPL
PB110979BS - 1	LCSW	14459	3.8108	-7470A	PPB		11 Jul 2018 10:40:11	U	SMPL
PB110979TB - 1	PB110943TB	186	-0.0057	-7470A	PPB		11 Jul 2018 10:42:19	U	SMPL
J3827-02 - 1	OR-03-070918	279	0.0191	-7470A	PPB		11 Jul 2018 10:44:27	U	SMPL
J3827-02DUP - 1	OR-03-070918DUP	252	0.0119	-7470A	PPB		11 Jul 2018 10:46:36	U	SMPL
J3827-02MS - 1	OR-03-070918MS	14117	3.7194	-7470A	PPB		11 Jul 2018 10:48:44	U	SMPL
J3827-02MSD - 1	OR-03-070918MSD	13687	3.6044	-7470A	PPB		11 Jul 2018 10:50:50	U	SMPL
CCV48 - 1	CCV48	18645	4.9302	-7470A	PPB		11 Jul 2018 10:52:58	U	SMPL
CCB48 - 1	CCB48	177	-0.0081	-7470A	PPB		11 Jul 2018 10:57:50	U	SMPL
J3903-02 - 1	KS-T-1	363	0.0416	-7470A	PPB		11 Jul 2018 10:59:56	U	SMPL
J3903-04 - 1	KS-T-3	416	0.0558	-7470A	PPB		11 Jul 2018 11:02:03	U	SMPL
J3908-04 - 1	TP-10-S	513	0.0817	-7470A	PPB		11 Jul 2018 11:04:10	U	SMPL
J3912-01 - 1	GS-CON	313	0.0282	-7470A	PPB		11 Jul 2018 11:06:17	U	SMPL
J3912-02 - 1	GS-CONCRETE-PIPE	93	-0.0306	-7470A	PPB		11 Jul 2018 11:08:24	U	SMPL
J3914-02 - 1	B1	224	0.0044	-7470A	PPB		11 Jul 2018 11:10:31	U	SMPL
J3914-04 - 1	B2	282	0.0199	-7470A	PPB		11 Jul 2018 11:12:39	U	SMPL
J3914-06 - 1	B3	297	0.0239	-7470A	PPB		11 Jul 2018 11:14:47	U	SMPL
J3914-08 - 1	NEMH	280	0.0194	-7470A	PPB		11 Jul 2018 11:16:56	U	SMPL
J3914-10 - 1	SEMh	299	0.0245	-7470A	PPB		11 Jul 2018 11:19:03	U	SMPL
CCV49 - 1	CCV49	18685	4.9409	-7470A	PPB		11 Jul 2018 11:21:10	U	SMPL
CCB49 - 1	CCB49	52	-0.0416	-7470A	PPB		11 Jul 2018 11:23:17	U	SMPL
J3914-12 - 1	SMH	286	0.0210	-7470A	PPB		11 Jul 2018 11:25:25	U	SMPL
PB110980BL - 1	PBW	220	0.0033	-7470A	PPB		11 Jul 2018 11:27:31	U	SMPL
PB110980BS - 1	LCSW	13768	3.6261	-7470A	PPB		11 Jul 2018 11:29:39	U	SMPL
PB110980TB - 1	PB110946TB	126	-0.0218	-7470A	PPB		11 Jul 2018 11:31:46	U	SMPL
J3911-02 - 1	RB47196RT	304	0.0258	-7470A	PPB		11 Jul 2018 11:33:53	U	SMPL
J3911-04 - 1	VB21029	448	0.0643	-7470A	PPB		11 Jul 2018 11:36:01	U	SMPL
J3911-04DUP - 1	VB21029DUP	492	0.0761	-7470A	PPB		11 Jul 2018 11:38:08	U	SMPL
J3911-04MS - 1	VB21029MS	14869	3.9205	-7470A	PPB		11 Jul 2018 11:40:17	U	SMPL
J3911-04MSD - 1	VB21029MSD	15101	3.9825	-7470A	PPB		11 Jul 2018 11:42:25	U	SMPL
PB110981BL - 1	PBW	143	-0.0172	-7470A	PPB		11 Jul 2018 11:44:33	U	SMPL
CCV50 - 1	CCV50	19086	5.0481	-7470A	PPB		11 Jul 2018 11:46:40	U	SMPL
CCB50 - 1	CCB50	102	-0.0282	-7470A	PPB		11 Jul 2018 11:48:47	U	SMPL
PB110981BS - 1	LCSW	13786	3.6309	-7470A	PPB		11 Jul 2018 11:50:55	U	SMPL
J3911-01 - 1	RB47196RT	54689	14.5683	-7470A	PPB		11 Jul 2018 11:53:02	U	SMPL
J3911-01DUP - 1	RB47196RTDUP	54141	14.4218	-7470A	PPB		11 Jul 2018 11:55:08	U	SMPL
J3911-01MS - 1	RB47196RTMS	67083	17.8825	-7470A	PPB		11 Jul 2018 11:57:19	U	SMPL
J3911-01MSD - 1	RB47196RTMSD	68567	18.2793	-7470A	PPB		11 Jul 2018 11:59:29	U	SMPL
J3911-03 - 1	VB21029	38265	10.1765	-7470A	PPB		11 Jul 2018 12:01:39	U	SMPL
J3928-03 - 1	GROUNDWATER	75	-0.0354	-7470A	PPB		11 Jul 2018 12:06:32	U	SMPL
J3827-02LX5 - 1		2	-0.0549	-7470A	PPB		11 Jul 2018 12:08:40	U	SMPL
J3827-02A - 1		14557	3.8371	-7470A	PPB		11 Jul 2018 12:10:48	U	SMPL
J3911-04LX5 - 1		388	0.0483	-7470A	PPB		11 Jul 2018 12:12:55	U	SMPL
CCV51 - 1	CCV51	19048	5.0379	-7470A	PPB		11 Jul 2018 12:15:02	U	SMPL
CCB51 - 1	CCB51	99	-0.0290	-7470A	PPB		11 Jul 2018 12:17:09	U	SMPL
J3911-04A - 1		14402	3.7956	-7470A	PPB		11 Jul 2018 12:19:17	U	SMPL
J3911-01LX5 - 1		11259	2.9552	-7470A	PPB		11 Jul 2018 12:25:33	U	SMPL
J3911-01A - 1		67929	18.1087	-7470A	PPB		11 Jul 2018 12:27:40	U	SMPL
J3911-01DLX5 - 1		11140	2.9233	-7470A	PPB		11 Jul 2018 12:29:47	U	SMPL
J3911-01DUPDLX5 - 1		11394	2.9913	-7470A	PPB		11 Jul 2018 12:31:56	U	SMPL
J3911-01MSDLX5 - 1		13921	3.6670	-7470A	PPB		11 Jul 2018 12:34:04	U	SMPL
J3911-01MSDDLX5 - 1		13978	3.6822	-7470A	PPB		11 Jul 2018 12:36:12	U	SMPL
J3911-01LDLX25 - 1		2294	0.5579	-7470A	PPB		11 Jul 2018 12:38:20	U	SMPL
J3911-01ADLX5 - 1		14538	3.8320	-7470A	PPB		11 Jul 2018 12:40:29	U	SMPL
J3911-03DLX2 - 1		19938	5.2759	-7470A	PPB		11 Jul 2018 12:42:36	U	SMPL
CCV52 - 1	CCV52	18981	5.0200	-7470A	PPB		11 Jul 2018 12:44:44	U	SMPL
CCB52 - 1	CCB52	108	-0.0266	-7470A	PPB		11 Jul 2018 12:46:52	U	SMPL