


7471B

LB 96568
INSTRUMENT ID: CV2

Linear

 μ Abs.:

44530

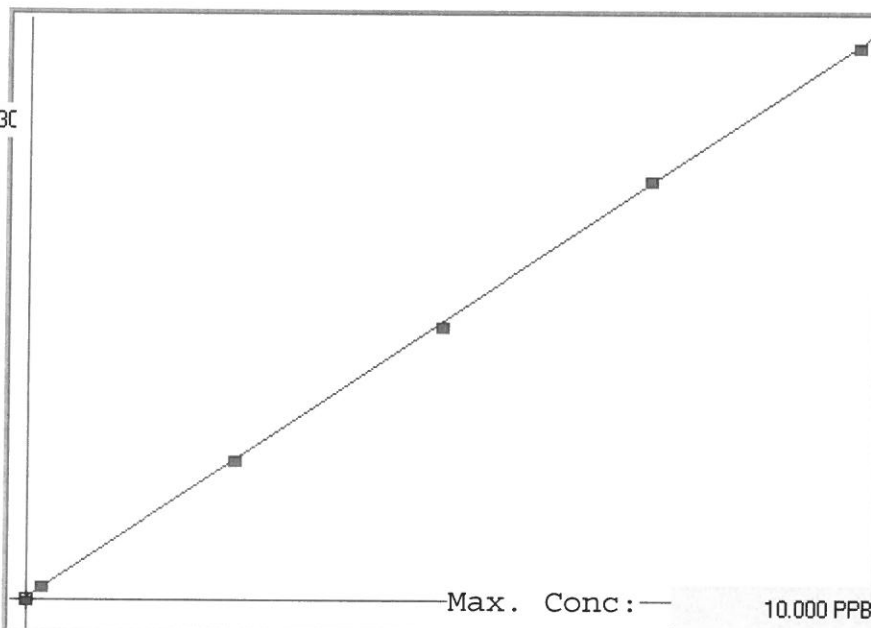

A= 0.0000e+000

B= 2.2475e-004

C= -3.0930e-002

Rho= 0.9999308

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.022	-0.022	41	0.000	41				
0.2	0.200	0.234	0.034	1181	0.0 %	1181				
2.5	2.500	2.506	0.006	11286	0.0 %	11286				
5.0	5.000	4.935	-0.065	22095	0.0 %	22095				
7.5	7.500	7.570	0.070	33818	0.0 %	33818				
10.0	10.000	9.977	-0.023	44530	0.0 %	44530				

LB96568 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 11 Jul 2018 15:37:48

Sample ID	Extended ID	μ Abs	Conc	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	41	-	0.0007471B	PPB		11 Jul 2018 15:40:55	S	Std
0.2 - 1	50.2	1181	-	0.20007471B	PPB		11 Jul 2018 15:43:12	S	Std
2.5 - 1	52.5	11286	-	2.50007471B	PPB		11 Jul 2018 15:45:31	S	Std
5.0 - 1	55	22095	-	5.00007471B	PPB		11 Jul 2018 15:47:48	S	Std
7.5 - 1	57.5	33818	-	7.50007471B	PPB		11 Jul 2018 15:50:05	S	Std
10.0 - 1	510	44530	-	10.00007471B	PPB		11 Jul 2018 15:52:22	S	Std
ICV44 - 1	ICV44	18085	4.0336	-7471B	PPB		11 Jul 2018 15:55:18	U	SMPL
ICB44 - 1	ICB44	-3	-0.0316	-7471B	PPB		11 Jul 2018 15:57:33	U	SMPL
CCV53 - 1	CCV53	22245	4.9686	-7471B	PPB		11 Jul 2018 15:59:49	U	SMPL
CCB53 - 1	CCB53	-1	-0.0312	-7471B	PPB		11 Jul 2018 16:02:05	U	SMPL
CRA - 1	CRA	1173	0.2327	-7471B	PPB		11 Jul 2018 16:04:21	U	SMPL
HighStd - 1	HighStd	44736	10.0234	-7471B	PPB		11 Jul 2018 16:06:37	U	SMPL
ChkStd - 1	ChkStd	31336	7.0118	-7471B	PPB		11 Jul 2018 16:08:53	U	SMPL
PB110985BL - 1	PBS	-127	-0.0595	-7471B	PPB		11 Jul 2018 16:11:11	U	SMPL
PB110985BS - 1	LCSS	16475	3.6718	-7471B	PPB		11 Jul 2018 16:13:29	U	SMPL
J3824-01 - 1	HD-02-071018	2524	0.5363	-7471B	PPB		11 Jul 2018 16:15:46	U	SMPL
J3828-01 - 1	EO-01-071018-A	2147	0.4516	-7471B	PPB		11 Jul 2018 16:18:04	U	SMPL
J3828-03 - 1	EO-01-071018-B	2545	0.5411	-7471B	PPB		11 Jul 2018 16:20:21	U	SMPL
J3828-05 - 1	EO-01-071018-C	1401	0.2839	-7471B	PPB		11 Jul 2018 16:22:39	U	SMPL
J3832-01 - 1	TR-05-071018	1501	0.3064	-7471B	PPB		11 Jul 2018 16:24:55	U	SMPL
CCV54 - 1	CCV54	21881	4.8868	-7471B	PPB		11 Jul 2018 16:27:11	U	SMPL
CCB54 - 1	CCB54	-3	-0.0316	-7471B	PPB		11 Jul 2018 16:29:27	U	SMPL
J3918-01 - 1	VNJ-204-255-ETS	32184	7.2024	-7471B	PPB		11 Jul 2018 16:31:44	U	SMPL
J3924-01 - 1	RO-1-4	80508	18.0631	-7471B	PPB		11 Jul 2018 16:34:00	U	SMPL
J3926-01 - 1	TRAP-BAG	162	0.0055	-7471B	PPB		11 Jul 2018 16:38:56	U	SMPL
J3927-01 - 1	CS-RBR-200031	8145	1.7996	-7471B	PPB		11 Jul 2018 16:41:12	U	SMPL
J3929-01 - 1	EPE-MX-6(5-27)-COMPOSITE	183	0.0102	-7471B	PPB		11 Jul 2018 16:43:29	U	SMPL
J3929-02 - 1	EPE-MX-6(30-52)-COMPOSITE	159	0.0048	-7471B	PPB		11 Jul 2018 16:45:45	U	SMPL
J3929-03 - 1	EPE-MX-6(55-77)-COMPOSITE	428	0.0653	-7471B	PPB		11 Jul 2018 16:48:03	U	SMPL
J3930-01 - 1	NYS-RBR-200030	1398	0.2833	-7471B	PPB		11 Jul 2018 16:50:20	U	SMPL
J3930-01DUP - 1	NYS-RBR-200030DUP	1318	0.2653	-7471B	PPB		11 Jul 2018 16:52:38	U	SMPL
J3930-01MS - 1	NYS-RBR-200030MS	19968	4.4569	-7471B	PPB		11 Jul 2018 16:57:35	U	SMPL
CCV55 - 1	CCV55	22074	4.9302	-7471B	PPB		11 Jul 2018 16:59:51	U	SMPL
CCB55 - 1	CCB55	-33	-0.0383	-7471B	PPB		11 Jul 2018 17:02:07	U	SMPL
J3930-01MSD - 1	NYS-RBR-200030MSD	18542	4.1364	-7471B	PPB		11 Jul 2018 17:04:24	U	SMPL
J3930-01LX5 - 1		159	0.0048	-7471B	PPB		11 Jul 2018 17:06:40	U	SMPL
J3930-01A - 1		19775	4.4135	-7471B	PPB		11 Jul 2018 17:08:56	U	SMPL
J3924-01DLX5 - 1		15631	3.4821	-7471B	PPB		11 Jul 2018 17:11:13	U	SMPL
CCV56 - 1	CCV56	22107	4.9376	-7471B	PPB		11 Jul 2018 17:13:29	U	SMPL
CCB56 - 1	CCB56	-11	-0.0334	-7471B	PPB		11 Jul 2018 17:15:47	U	SMPL