

LB 96625


7470A

INSTRUMENT ID: CV1

Linear

 μ Abs.:

3811E

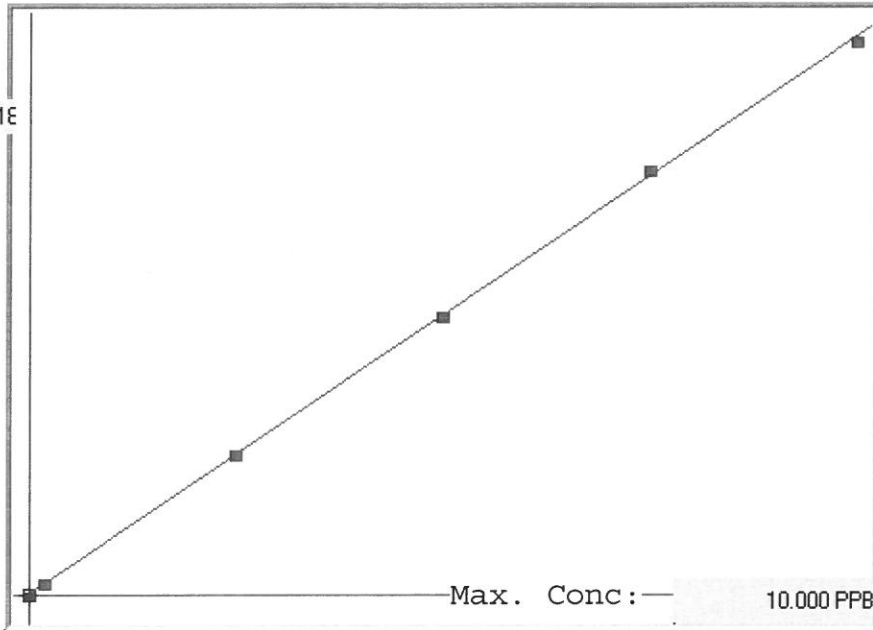

A= 0.0000e+000

B= 2.6088e-004

C= -1.6052e-002

Rho= 0.9998976

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.029	-0.029	-48	0.000	-48				
0.2	0.200	0.204	0.004	843	0.0 %	843				
2.5	2.500	2.514	0.014	9697	0.0 %	9697				
5.0	5.000	4.982	-0.018	19158	0.0 %	19158				
7.5	7.500	7.601	0.101	29198	0.0 %	29198				
10.0	10.000	9.928	-0.072	38118	0.0 %	38118				

LB96625 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 13 Jul 2018 09:12:45

Sample ID	Extended ID	μ Abs	Conc	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-48	-	0.000	7470A	PPB	13 Jul 2018 09:19:13	S	Std
0.2 - 1	502	843	-	0.200	7470A	PPB	13 Jul 2018 09:21:21	S	Std
2.5 - 1	52.5	9697	-	2.500	7470A	PPB	13 Jul 2018 09:23:29	S	Std
5.0 - 1	55	19158	-	5.000	7470A	PPB	13 Jul 2018 09:25:38	S	Std
7.5 - 1	57.5	29198	-	7.500	7470A	PPB	13 Jul 2018 09:27:46	S	Std
10.0 - 1	510	38118	-	10.000	7470A	PPB	13 Jul 2018 09:32:19	S	Std
ICV48 - 1	ICV48	14704	3.8199	-7470A	PPB	PPB	13 Jul 2018 09:34:56	U	SMPL
ICB48 - 1	ICB48	-178	-0.0625	-7470A	PPB	PPB	13 Jul 2018 09:37:02	U	SMPL
CCV70 - 1	CCV70	19496	5.0700	-7470A	PPB	PPB	13 Jul 2018 09:39:09	U	SMPL
CCB70 - 1	CCB70	-181	-0.0633	-7470A	PPB	PPB	13 Jul 2018 09:41:15	U	SMPL
CRA - 1	CRA	830	0.2005	-7470A	PPB	PPB	13 Jul 2018 09:43:22	U	SMPL
HighStd - 1	HighStd	38688	10.0768	-7470A	PPB	PPB	13 Jul 2018 09:45:29	U	SMPL
ChkStd - 1	ChkStd	26651	6.9366	-7470A	PPB	PPB	13 Jul 2018 09:47:35	U	SMPL
PB111064BL - 1	PBW	-275	-0.0878	-7470A	PPB	PPB	13 Jul 2018 09:49:45	U	SMPL
PB111064BS - 1	LCSW	12941	3.3600	-7470A	PPB	PPB	13 Jul 2018 09:51:53	U	SMPL
PB111064TB - 1	PB111017TB	-150	-0.0552	-7470A	PPB	PPB	13 Jul 2018 09:54:01	U	SMPL
J3825-02 - 1	CL-02-071118-A	-76	-0.0359	-7470A	PPB	PPB	13 Jul 2018 09:56:09	U	SMPL
J3825-02DUP - 1	CL-02-071118-ADUP	-58	-0.0312	-7470A	PPB	PPB	13 Jul 2018 09:58:17	U	SMPL
J3825-02MS - 1	CL-02-071118-AMS	13450	3.4928	-7470A	PPB	PPB	13 Jul 2018 10:00:25	U	SMPL
J3825-02MSD - 1	CL-02-071118-AMSD	12882	3.3446	-7470A	PPB	PPB	13 Jul 2018 10:02:32	U	SMPL
CCV71 - 1	CCV71	19337	5.0285	-7470A	PPB	PPB	13 Jul 2018 10:04:39	U	SMPL
CCB71 - 1	CCB71	-200	-0.0682	-7470A	PPB	PPB	13 Jul 2018 10:06:45	U	SMPL
J3825-04 - 1	CL-02-071118-B	-79	-0.0367	-7470A	PPB	PPB	13 Jul 2018 10:08:53	U	SMPL
J3825-06 - 1	CL-02-071118-C	-51	-0.0294	-7470A	PPB	PPB	13 Jul 2018 10:11:00	U	SMPL
J3825-08 - 1	CL-02-071118-D	-36	-0.0254	-7470A	PPB	PPB	13 Jul 2018 10:13:06	U	SMPL
J3825-10 - 1	CL-02-071118-E	-78	-0.0364	-7470A	PPB	PPB	13 Jul 2018 10:15:13	U	SMPL
J3929-01 - 1	EPE-MX-6(5-27)-COMPOSITE	-86	-0.0385	-7470A	PPB	PPB	13 Jul 2018 10:17:21	U	SMPL
J3929-02 - 1	EPE-MX-6(30-52)-COMPOSITE	-96	-0.0411	-7470A	PPB	PPB	13 Jul 2018 10:19:28	U	SMPL
J3929-03 - 1	EPE-MX-6(55-77)-COMPOSITE	-46	-0.0281	-7470A	PPB	PPB	13 Jul 2018 10:21:36	U	SMPL
J3948-02 - 1	2018-NYSEG-CLARK-ST-PH4-AREA-2-BANK	-76	-0.0359	-7470A	PPB	PPB	13 Jul 2018 10:23:45	U	SMPL
J3948-04 - 1	2018-NYSEG-CLARK-ST-PH4-AREA-3-BANK	-68	-0.0338	-7470A	PPB	PPB	13 Jul 2018 10:25:53	U	SMPL
J3948-06 - 1	2018-NYSEG-CLARK-ST-PH4-AREA-5-6-BANK	-69	-0.0341	-7470A	PPB	PPB	13 Jul 2018 10:28:00	U	SMPL
CCV72 - 1	CCV72	19380	5.0398	-7470A	PPB	PPB	13 Jul 2018 10:30:07	U	SMPL
CCB72 - 1	CCB72	-171	-0.0607	-7470A	PPB	PPB	13 Jul 2018 10:32:14	U	SMPL
PB111065BL - 1	PBW	-55	-0.0304	-7470A	PPB	PPB	13 Jul 2018 10:34:22	U	SMPL
PB111065BS - 1	LCSW	13752	3.5715	-7470A	PPB	PPB	13 Jul 2018 10:36:29	U	SMPL
PB111065TB - 1	PB111019TB	-156	-0.0567	-7470A	PPB	PPB	13 Jul 2018 10:38:36	U	SMPL
J3947-02 - 1	PAR-1	-101	-0.0424	-7470A	PPB	PPB	13 Jul 2018 10:40:43	U	SMPL
J3947-02DUP - 1	PAR-1DUP	-68	-0.0338	-7470A	PPB	PPB	13 Jul 2018 10:42:50	U	SMPL
J3947-02MS - 1	PAR-1MS	12521	3.2504	-7470A	PPB	PPB	13 Jul 2018 10:44:58	U	SMPL
J3947-02MSD - 1	PAR-1MSD	12720	3.3023	-7470A	PPB	PPB	13 Jul 2018 10:47:06	U	SMPL
J3947-04 - 1	PAR-2	71	0.0025	-7470A	PPB	PPB	13 Jul 2018 10:49:15	U	SMPL
J3947-06 - 1	PAR-3	-71	-0.0346	-7470A	PPB	PPB	13 Jul 2018 10:51:23	U	SMPL
J3947-08 - 1	PAR-4	-8	-0.0181	-7470A	PPB	PPB	13 Jul 2018 10:53:30	U	SMPL
CCV73 - 1	CCV73	19263	5.0092	-7470A	PPB	PPB	13 Jul 2018 10:55:38	U	SMPL
CCB73 - 1	CCB73	-235	-0.0774	-7470A	PPB	PPB	13 Jul 2018 10:57:45	U	SMPL
PB111066BL - 1	PBW	-56	-0.0307	-7470A	PPB	PPB	13 Jul 2018 10:59:53	U	SMPL
PB111066BS - 1	LCSW	13518	3.5105	-7470A	PPB	PPB	13 Jul 2018 11:02:00	U	SMPL
PB111066TB - 1	PB111023TB	-162	-0.0583	-7470A	PPB	PPB	13 Jul 2018 11:04:07	U	SMPL
J3934-02 - 1	TS-BASELINE-WATER	-79	-0.0367	-7470A	PPB	PPB	13 Jul 2018 11:06:14	U	SMPL
J3934-02DUP - 1	TS-BASELINE-WATERDUP	-47	-0.0283	-7470A	PPB	PPB	13 Jul 2018 11:08:22	U	SMPL
J3934-02MS - 1	TS-BASELINE-WATERMS	13446	3.4917	-7470A	PPB	PPB	13 Jul 2018 11:10:30	U	SMPL
J3934-02MSD - 1	TS-BASELINE-WATERMSD	13615	3.5358	-7470A	PPB	PPB	13 Jul 2018 11:12:38	U	SMPL
J3947-28 - 1	PAR-1-OILY-WATER	-183	-0.0638	-7470A	PPB	PPB	13 Jul 2018 11:14:46	U	SMPL
PB111076BL - 1	PBW	-39	-0.0262	-7470A	PPB	PPB	13 Jul 2018 11:16:55	U	SMPL
PB111076BS - 1	LCSW	13196	3.4265	-7470A	PPB	PPB	13 Jul 2018 11:19:02	U	SMPL
CCV74 - 1	CCV74	19138	4.9766	-7470A	PPB	PPB	13 Jul 2018 11:21:09	U	SMPL
CCB74 - 1	CCB74	-204	-0.0693	-7470A	PPB	PPB	13 Jul 2018 11:23:17	U	SMPL
J3947-27 - 1	PAR-1-OILY-WATER	11639	3.0203	-7470A	PPB	PPB	13 Jul 2018 11:25:24	U	SMPL
J3947-27DUP - 1	PAR-1-OILY-WATERDUP	11270	2.9240	-7470A	PPB	PPB	13 Jul 2018 11:27:32	U	SMPL
J3947-27MS - 1	PAR-1-OILY-WATERMS	25696	6.6875	-7470A	PPB	PPB	13 Jul 2018 11:29:40	U	SMPL
J3947-27MSD - 1	PAR-1-OILY-WATERMSD	25923	6.7467	-7470A	PPB	PPB	13 Jul 2018 11:31:48	U	SMPL
J3959-01 - 1	WC-20180712	829	0.2002	-7470A	PPB	PPB	13 Jul 2018 11:33:56	U	SMPL
J3825-02LX5 - 1		-85	-0.0382	-7470A	PPB	PPB	13 Jul 2018 11:36:06	U	SMPL
J3825-02A - 1		13764	3.5747	-7470A	PPB	PPB	13 Jul 2018 11:38:13	U	SMPL
J3947-02LX5 - 1		-165	-0.0591	-7470A	PPB	PPB	13 Jul 2018 11:40:22	U	SMPL
J3947-02A - 1		14261	3.7043	-7470A	PPB	PPB	13 Jul 2018 11:42:31	U	SMPL
CCV75 - 1	CCV75	19583	5.0927	-7470A	PPB	PPB	13 Jul 2018 11:44:38	U	SMPL
CCB75 - 1	CCB75	-189	-0.0654	-7470A	PPB	PPB	13 Jul 2018 11:46:46	U	SMPL
J3934-02LX5 - 1		-62	-0.0322	-7470A	PPB	PPB	13 Jul 2018 11:48:54	U	SMPL
J3934-02A - 1		13872	3.6028	-7470A	PPB	PPB	13 Jul 2018 11:51:01	U	SMPL
J3947-27LX5 - 1		1907	0.4814	-7470A	PPB	PPB	13 Jul 2018 11:53:09	U	SMPL
J3947-27A - 1		25624	6.6687	-7470A	PPB	PPB	13 Jul 2018 11:55:16	U	SMPL
CCV76 - 1	CCV76	19168	4.9845	-7470A	PPB	PPB	13 Jul 2018 11:57:24	U	SMPL
CCB76 - 1	CCB76	-216	-0.0724	-7470A	PPB	PPB	13 Jul 2018 11:59:32	U	SMPL