

7470A


L396656

INSTRUMENT ID: CV1

Linear

 μ Abs.:

38713

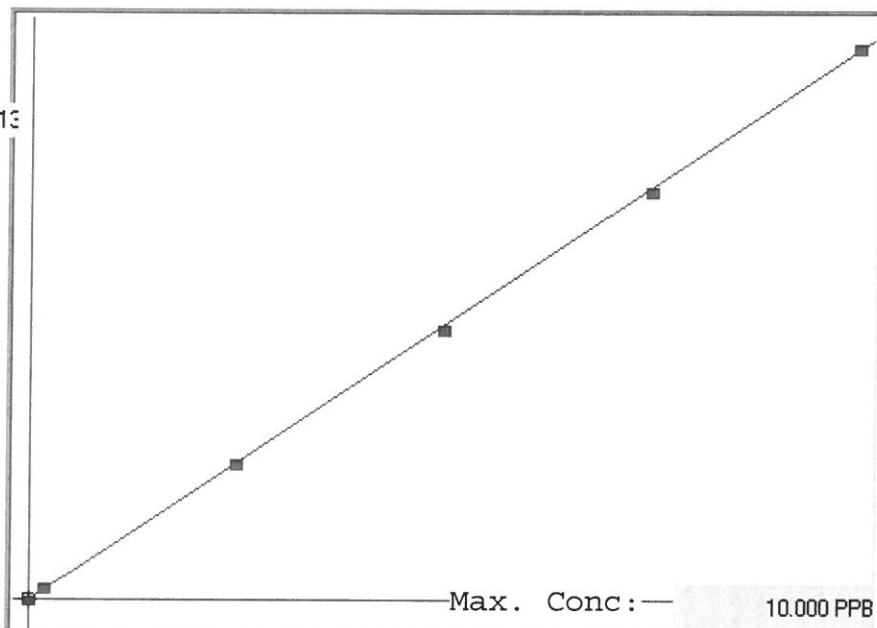

A= 0.0000e+000

B= 2.5907e-004

C= 2.2416e-002

Rho= 0.9999519

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.001	-0.001	-89	0.000	-89				
0.2	0.200	0.236	0.036	824	0.0 %	824				
2.5	2.500	2.500	0.000	9565	0.0 %	9565				
5.0	5.000	4.951	-0.049	19025	0.0 %	19025				
7.5	7.500	7.461	-0.039	28713	0.0 %	28713				
10.0	10.000	10.052	0.052	38713	0.0 %	38713				

LB96656 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 16 Jul 2018 09:04:40

Sample ID	Extended ID	μ Abs	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-89	-	0.0000	7470A	PPB	16 Jul 2018 09:40:07	S	Std
0.2 - 1	50.2	824	-	0.2000	7470A	PPB	16 Jul 2018 09:42:16	S	Std
2.5 - 1	52.5	9565	-	2.5000	7470A	PPB	16 Jul 2018 09:44:24	S	Std
5.0 - 1	55	19025	-	5.0000	7470A	PPB	16 Jul 2018 09:46:32	S	Std
7.5 - 1	57.5	28713	-	7.5000	7470A	PPB	16 Jul 2018 09:48:40	S	Std
10.0 - 1	57.0	38713	-	10.0000	7470A	PPB	16 Jul 2018 09:50:48	S	Std
ICV51 - 1	ICV51	14919	3.8875	-7470A	PPB	16 Jul 2018 09:53:27	U	SMPL	
ICB51 - 1	ICB51	-157	-0.0183	-7470A	PPB	16 Jul 2018 09:55:32	U	SMPL	
CCV88 - 1	CCV88	18706	4.8686	-7470A	PPB	16 Jul 2018 09:57:39	U	SMPL	
CCB88 - 1	CCB88	-181	-0.0245	-7470A	PPB	16 Jul 2018 09:59:46	U	SMPL	
CRA - 1	CRA	791	0.2273	-7470A	PPB	16 Jul 2018 10:01:53	U	SMPL	
HighStd - 1	HighStd	38861	10.0902	-7470A	PPB	16 Jul 2018 10:03:59	U	SMPL	
ChkStd - 1	ChkStd	27054	7.0314	-7470A	PPB	16 Jul 2018 10:06:06	U	SMPL	
PB111116BL - 1	PBW	186	0.0706	-7470A	PPB	16 Jul 2018 10:23:25	U	SMPL	
PB111116BS - 1	LCSW	14237	3.7108	-7470A	PPB	16 Jul 2018 10:25:32	U	SMPL	
PB111116TB - 1	PB111068TB	419	0.1310	-7470A	PPB	16 Jul 2018 10:27:40	U	SMPL	
J3542-04 - 1	LL-SOIL-1	430	0.1338	-7470A	PPB	16 Jul 2018 10:29:48	U	SMPL	
J3542-04DUP - 1	LL-SOIL-1DUP	441	0.1367	-7470A	PPB	16 Jul 2018 10:31:56	U	SMPL	
J3542-04MS - 1	LL-SOIL-1MS	14044	3.6608	-7470A	PPB	16 Jul 2018 10:34:05	U	SMPL	
J3542-04MSD - 1	LL-SOIL-1MSD	13314	3.4717	-7470A	PPB	16 Jul 2018 10:36:11	U	SMPL	
CCV89 - 1	CCV89	18689	4.8642	-7470A	PPB	16 Jul 2018 10:38:18	U	SMPL	
CCB89 - 1	CCB89	-186	-0.0258	-7470A	PPB	16 Jul 2018 10:40:24	U	SMPL	
J3542-08 - 1	LL-SOIL-2	352	0.1136	-7470A	PPB	16 Jul 2018 10:42:32	U	SMPL	
J3542-12 - 1	LL-SOIL-3	273	0.0931	-7470A	PPB	16 Jul 2018 10:44:38	U	SMPL	
J3545-01 - 1	DRUM-2	342	0.1110	-7470A	PPB	16 Jul 2018 10:46:45	U	SMPL	
J3545-04 - 1	DRUM-3	245	0.0859	-7470A	PPB	16 Jul 2018 10:48:51	U	SMPL	
J3820-04 - 1	BU-02-071218	-17	0.0180	-7470A	PPB	16 Jul 2018 10:50:59	U	SMPL	
J3821-02 - 1	HR-05-071218-A	492	0.1499	-7470A	PPB	16 Jul 2018 10:53:07	U	SMPL	
J3821-04 - 1	HR-05-071218-B	461	0.1418	-7470A	PPB	16 Jul 2018 10:55:14	U	SMPL	
J3821-06 - 1	HR-05-071218-C	538	0.1618	-7470A	PPB	16 Jul 2018 10:57:23	U	SMPL	
J3831-02 - 1	SU-04-071218	528	0.1592	-7470A	PPB	16 Jul 2018 10:59:31	U	SMPL	
J3958-06 - 1	CS-STONE	514	0.1556	-7470A	PPB	16 Jul 2018 11:01:38	U	SMPL	
CCV90 - 1	CCV90	18610	4.8438	-7470A	PPB	16 Jul 2018 11:03:45	U	SMPL	
CCB90 - 1	CCB90	-179	-0.0240	-7470A	PPB	16 Jul 2018 11:05:52	U	SMPL	
J3958-10 - 1	CS-CONCRETE	484	0.1478	-7470A	PPB	16 Jul 2018 11:07:59	U	SMPL	
J3966-03 - 1	72-11977	514	0.1556	-7470A	PPB	16 Jul 2018 11:10:06	U	SMPL	
J3975-02 - 1	PAR-5	635	0.1869	-7470A	PPB	16 Jul 2018 11:12:13	U	SMPL	
J3975-04 - 1	PAR-6	665	0.1947	-7470A	PPB	16 Jul 2018 11:14:20	U	SMPL	
J3975-06 - 1	PAR-7	665	0.1947	-7470A	PPB	16 Jul 2018 11:16:27	U	SMPL	
J3975-08 - 1	PAR-8	593	0.1760	-7470A	PPB	16 Jul 2018 11:18:35	U	SMPL	
J3980-04 - 1	TP-E-MH-S	536	0.1613	-7470A	PPB	16 Jul 2018 11:20:42	U	SMPL	
J3980-08 - 1	TP-E-MH-D	476	0.1457	-7470A	PPB	16 Jul 2018 11:22:51	U	SMPL	
PB111117BS - 1	LCSW	14152	3.6888	-7470A	PPB	16 Jul 2018 11:27:06	U	SMPL	
CCV91 - 1	CCV91	18264	4.7541	-7470A	PPB	16 Jul 2018 11:29:13	U	SMPL	
CCB91 - 1	CCB91	-190	-0.0268	-7470A	PPB	16 Jul 2018 11:31:20	U	SMPL	
PB111117TB - 1	PB111070TB	513	0.1553	-7470A	PPB	16 Jul 2018 11:33:28	U	SMPL	
J3545-06 - 1	DRUM-1	457	0.1408	-7470A	PPB	16 Jul 2018 11:35:35	U	SMPL	
J3954-02 - 1	FM1041	415	0.1299	-7470A	PPB	16 Jul 2018 11:37:41	U	SMPL	
J3959-02 - 1	WC-20180712	756	0.2183	-7470A	PPB	16 Jul 2018 11:39:49	U	SMPL	
J3959-02DUP - 1	WC-20180712DUP	769	0.2216	-7470A	PPB	16 Jul 2018 11:41:56	U	SMPL	
J3959-02MS - 1	WC-20180712MS	16992	4.4246	-7470A	PPB	16 Jul 2018 11:44:03	U	SMPL	
J3959-02MSD - 1	WC-20180712MSD	16649	4.3357	-7470A	PPB	16 Jul 2018 11:46:12	U	SMPL	
J3964-02 - 1	N48967	545	0.1636	-7470A	PPB	16 Jul 2018 11:48:20	U	SMPL	
J3975-14 - 1	SV30518L	525	0.1584	-7470A	PPB	16 Jul 2018 11:50:29	U	SMPL	
PB111118BL - 1	PBW	2	0.0229	-7470A	PPB	16 Jul 2018 11:55:08	U	SMPL	
CCV92 - 1	CCV92	18844	4.9044	-7470A	PPB	16 Jul 2018 11:57:15	U	SMPL	
CCB92 - 1	CCB92	-192	-0.0273	-7470A	PPB	16 Jul 2018 11:59:22	U	SMPL	
PB111118BS - 1	LCSW	12938	3.3743	-7470A	PPB	16 Jul 2018 12:01:29	U	SMPL	
PB111118TB - 1	PB111081TB	315	0.1040	-7470A	PPB	16 Jul 2018 12:03:36	U	SMPL	
J3956-02 - 1	CONTINGENCY-DUCK-BANK-CONCRETE-A	423	0.1320	-7470A	PPB	16 Jul 2018 12:11:41	U	SMPL	
J3956-02DUP - 1	CONTINGENCY-DUCK-BANK-CONCRETE-ADUP	406	0.1276	-7470A	PPB	16 Jul 2018 12:16:20	U	SMPL	
J3956-02MS - 1	CONTINGENCY-DUCK-BANK-CONCRETE-AMS	13562	3.5360	-7470A	PPB	16 Jul 2018 12:18:27	U	SMPL	
J3956-02MSD - 1	CONTINGENCY-DUCK-BANK-CONCRETE-AMSD	14869	3.8746	-7470A	PPB	16 Jul 2018 12:20:35	U	SMPL	
J3956-04 - 1	CONTINGENCY-DUCK-BANK-CONCRETE-B	499	0.1517	-7470A	PPB	16 Jul 2018 12:22:43	U	SMPL	
J3961-01 - 1	1-6-30-GAL-55-GAL-1-6	598	0.1773	-7470A	PPB	16 Jul 2018 12:24:51	U	SMPL	
J3961-02 - 1	DRUM-1	493	0.1501	-7470A	PPB	16 Jul 2018 12:27:00	U	SMPL	
J3961-03 - 1	DRUM-2	575	0.1714	-7470A	PPB	16 Jul 2018 12:29:07	U	SMPL	
CCV93 - 1	CCV93	18715	4.8710	-7470A	PPB	16 Jul 2018 12:31:14	U	SMPL	
CCB93 - 1	CCB93	-157	-0.0183	-7470A	PPB	16 Jul 2018 12:33:22	U	SMPL	
PB111119BL - 1	PBW	-114	-0.0071	-7470A	PPB	16 Jul 2018 12:35:29	U	SMPL	
PB111119BS - 1	LCSW	15016	3.9126	-7470A	PPB	16 Jul 2018 12:37:36	U	SMPL	
J3545-05 - 1	DRUM-1	33	0.0310	-7470A	PPB	16 Jul 2018 12:39:43	U	SMPL	
J3545-05DUP - 1	DRUM-1DUP	61	0.0382	-7470A	PPB	16 Jul 2018 12:41:51	U	SMPL	
J3545-05MS - 1	DRUM-1MS	13839	3.6077	-7470A	PPB	16 Jul 2018 12:43:58	U	SMPL	
J3545-05MSD - 1	DRUM-1MSD	13959	3.6388	-7470A	PPB	16 Jul 2018 12:46:06	U	SMPL	
J3954-01 - 1	FM1041	-94	-0.0019	-7470A	PPB	16 Jul 2018 12:48:15	U	SMPL	
J3964-01 - 1	N48967	291	0.0978	-7470A	PPB	16 Jul 2018 12:50:24	U	SMPL	
J3975-13 - 1	SV30518L	312	0.1032	-7470A	PPB	16 Jul 2018 12:52:33	U	SMPL	
PB111117BL - 1	PBW	40	0.0328	-7470A	PPB	16 Jul 2018 12:54:40	U	SMPL	
CCV94 - 1	CCV94	17747	4.6202	-7470A	PPB	16 Jul 2018 13:06:24	U	SMPL	
CCB94 - 1	CCB94	-146	-0.0154	-7470A	PPB	16 Jul 2018 13:08:31	U	SMPL	
J3542-04LX5 - 1		-15	0.0185	-7470A	PPB	16 Jul 2018 13:10:40	U	SMPL	
J3542-04A - 1		13807	3.5994	-7470A	PPB	16 Jul 2018 13:12:47	U	SMPL	
J3959-02LX5 - 1		-75	0.0030	-7470A	PPB	16 Jul 2018 13:14:55	U	SMPL	
J3959-02A - 1		15547	4.0502	-7470A	PPB	16 Jul 2018 13:17:03	U	SMPL	
J3956-02LX5 - 1		-125	-0.0100	-7470A	PPB	16 Jul 2018 13:19:11	U	SMPL	
J3956-02A - 1		13729	3.5792	-7470A	PPB	16 Jul 2018 13:21:19	U	SMPL	
J3545-05LX5 - 1		-158	-0.0185	-7470A	PPB	16 Jul 2018 13:23:27	U	SMPL	
J3545-05A - 1		12975	3.3839	-7470A	PPB	16 Jul 2018 13:25:35	U	SMPL	
J3941-01 - 1	SES-MS-PH4-COA-7-18	-324	-0.0615	-7470A	PPB	16 Jul 2018 13:27:43	U	SMPL	
CCV95 - 1	CCV95	18257	4.7523	-7470A	PPB	16 Jul 2018 13:29:51	U	SMPL	
CCB95 - 1	CCB95	-213	-0.0328	-7470A	PPB	16 Jul 2018 13:31:59	U	SMPL	