


7470A

LB 96689
INSTRUMENT ID: CV1

Linear

 μ Abs.:

39791

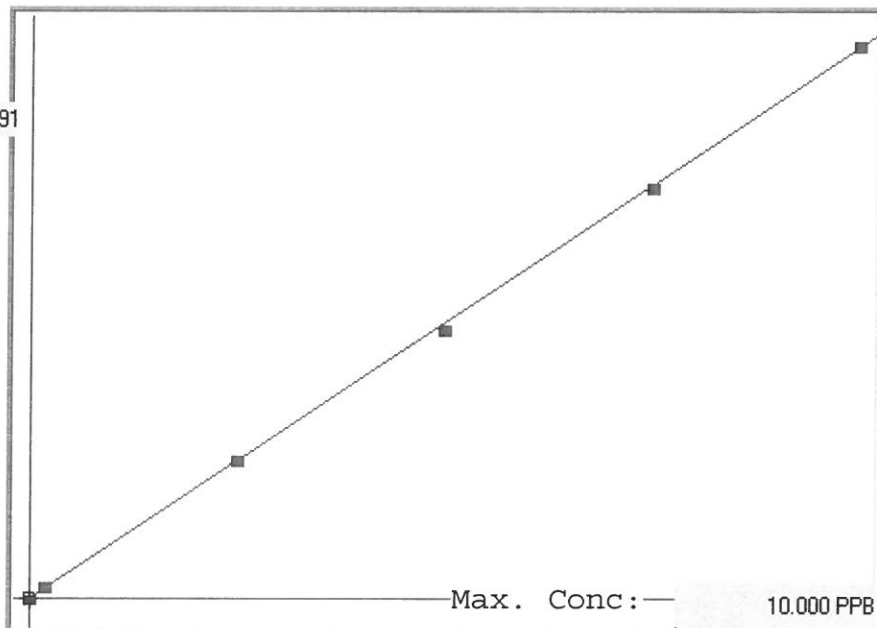

A= 0.0000e+000

B= 2.5262e-004

C= 5.7328e-003

Rho= 0.9998996

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.000	-0.000	-24	0.000	-24				
0.2	0.200	0.227	0.027	875	0.0 %	875				
2.5	2.500	2.543	0.043	10043	0.0 %	10043				
5.0	5.000	4.902	-0.098	19380	0.0 %	19380				
7.5	7.500	7.471	-0.029	29553	0.0 %	29553				
10.0	10.000	10.058	0.058	39791	0.0 %	39791				

LB96689 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 17 Jul 2018 12:21:19

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	SD	-24	-	0.00007470A	PPB		17 Jul 2018 12:25:04	S	Std
0.2 - 1	SD-2	875	-	0.20007470A	PPB		17 Jul 2018 12:27:12	S	Std
2.5 - 1	SD-5	10043	-	2.50007470A	PPB		17 Jul 2018 12:29:21	S	Std
5.0 - 1	SD	19380	-	5.00007470A	PPB		17 Jul 2018 12:31:29	S	Std
7.5 - 1	SD-5	29553	-	7.50007470A	PPB		17 Jul 2018 12:33:37	S	Std
10.0 - 1	SD	39791	-	10.00007470A	PPB		17 Jul 2018 12:35:45	S	Std
ICV54 - 1	ICV54	15039	3.8049	-7470A	PPB		17 Jul 2018 12:40:43	U	SMPL
ICB54 - 1	ICB54	-179	-0.0395	-7470A	PPB		17 Jul 2018 12:42:49	U	SMPL
CCV08 - 1	CCV08	19667	4.9740	-7470A	PPB		17 Jul 2018 12:44:56	U	SMPL
CCB08 - 1	CCB08	-193	-0.0430	-7470A	PPB		17 Jul 2018 12:47:02	U	SMPL
CRA - 1	CRA	885	0.2293	-7470A	PPB		17 Jul 2018 12:49:09	U	SMPL
HighStd - 1	HighStd	40248	10.1732	-7470A	PPB		17 Jul 2018 12:51:15	U	SMPL
ChkStd - 1	ChkStd	26360	6.6648	-7470A	PPB		17 Jul 2018 12:53:22	U	SMPL
PB111152BL - 1	PBW	-304	-0.0711	-7470A	PPB		17 Jul 2018 12:55:30	U	SMPL
PB111152BS - 1	LCSW	13398	3.3903	-7470A	PPB		17 Jul 2018 12:57:39	U	SMPL
PB111152TB - 1	PB111122TB	-140	-0.0296	-7470A	PPB		17 Jul 2018 12:59:47	U	SMPL
J3819-02 - 1	AU-05-071318-A	-20	0.0007	-7470A	PPB		17 Jul 2018 13:01:55	U	SMPL
J3819-02DUP - 1	AU-05-071318-ADUP	2	0.0062	-7470A	PPB		17 Jul 2018 13:04:03	U	SMPL
J3819-02MS - 1	AU-05-071318-AMS	13254	3.3540	-7470A	PPB		17 Jul 2018 13:06:12	U	SMPL
J3819-02MSD - 1	AU-05-071318-AMSD	14165	3.5841	-7470A	PPB		17 Jul 2018 13:08:18	U	SMPL
CCV09 - 1	CCV09	19532	4.9399	-7470A	PPB		17 Jul 2018 13:10:25	U	SMPL
CCB09 - 1	CCB09	-154	-0.0332	-7470A	PPB		17 Jul 2018 13:12:32	U	SMPL
J3819-04 - 1	AU-05-071318-B	-58	-0.0089	-7470A	PPB		17 Jul 2018 13:14:40	U	SMPL
J3819-06 - 1	AU-05-071318-C	1	0.0060	-7470A	PPB		17 Jul 2018 13:16:47	U	SMPL
J3819-08 - 1	AU-05-071318-D	-48	-0.0064	-7470A	PPB		17 Jul 2018 13:18:53	U	SMPL
J3829-02 - 1	PL-01-071318-A	-14	0.0022	-7470A	PPB		17 Jul 2018 13:21:00	U	SMPL
J3829-04 - 1	PL-01-071318-B	-15	0.0019	-7470A	PPB		17 Jul 2018 13:23:08	U	SMPL
J3829-06 - 1	PL-01-071318-C	-51	-0.0072	-7470A	PPB		17 Jul 2018 13:25:15	U	SMPL
J3996-06 - 1	MH-1	1	0.0060	-7470A	PPB		17 Jul 2018 13:27:23	U	SMPL
J3997-04 - 1	TP-F-S	-24	-0.0003	-7470A	PPB		17 Jul 2018 13:29:32	U	SMPL
J3997-08 - 1	TP-F-D	-2	0.0052	-7470A	PPB		17 Jul 2018 13:31:40	U	SMPL
J3997-12 - 1	TP-H-S	9	0.0080	-7470A	PPB		17 Jul 2018 13:33:47	U	SMPL
CCV10 - 1	CCV10	19528	4.9389	-7470A	PPB		17 Jul 2018 13:35:54	U	SMPL
CCB10 - 1	CCB10	-145	-0.0309	-7470A	PPB		17 Jul 2018 13:38:01	U	SMPL
J3997-16 - 1	TP-H-D	1	0.0060	-7470A	PPB		17 Jul 2018 13:40:09	U	SMPL
PB111175BL - 1	PBW	-16	0.0017	-7470A	PPB		17 Jul 2018 13:42:16	U	SMPL
PB111175BS - 1	LCSW	14106	3.5692	-7470A	PPB		17 Jul 2018 13:44:22	U	SMPL
J3993-01 - 1	20180414-FIELDBLANK	-254	-0.0584	-7470A	PPB		17 Jul 2018 13:46:29	U	SMPL
J4006-01 - 1	RR-BASELINE-WATER	-86	-0.0160	-7470A	PPB		17 Jul 2018 13:48:37	U	SMPL
J4008-01 - 1	KG-FM1026	-115	-0.0233	-7470A	PPB		17 Jul 2018 13:50:44	U	SMPL
J4008-01DUP - 1	KG-FM1026DUP	-109	-0.0218	-7470A	PPB		17 Jul 2018 13:52:52	U	SMPL
J4008-01MS - 1	KG-FM1026MS	14608	3.6960	-7470A	PPB		17 Jul 2018 13:55:01	U	SMPL
J4008-01MSD - 1	KG-FM1026MSD	14806	3.7460	-7470A	PPB		17 Jul 2018 13:57:09	U	SMPL
CCV11 - 1	CCV11	19778	5.0021	-7470A	PPB		17 Jul 2018 13:59:16	U	SMPL
CCB11 - 1	CCB11	-137	-0.0289	-7470A	PPB		17 Jul 2018 14:01:23	U	SMPL
J3819-02LX5 - 1		-42	-0.0049	-7470A	PPB		17 Jul 2018 14:03:32	U	SMPL
J3819-02A - 1		14672	3.7122	-7470A	PPB		17 Jul 2018 14:05:39	U	SMPL
J4008-01LX5 - 1		-88	-0.0165	-7470A	PPB		17 Jul 2018 14:09:33	U	SMPL
J4008-01A - 1		15059	3.8100	-7470A	PPB		17 Jul 2018 14:11:42	U	SMPL
CCV12 - 1	CCV12	19229	4.8634	-7470A	PPB		17 Jul 2018 14:13:49	U	SMPL
CCB12 - 1	CCB12	-215	-0.0486	-7470A	PPB		17 Jul 2018 14:15:57	U	SMPL