


L396926

7470A

INSTRUMENT ID: CV1

Linear

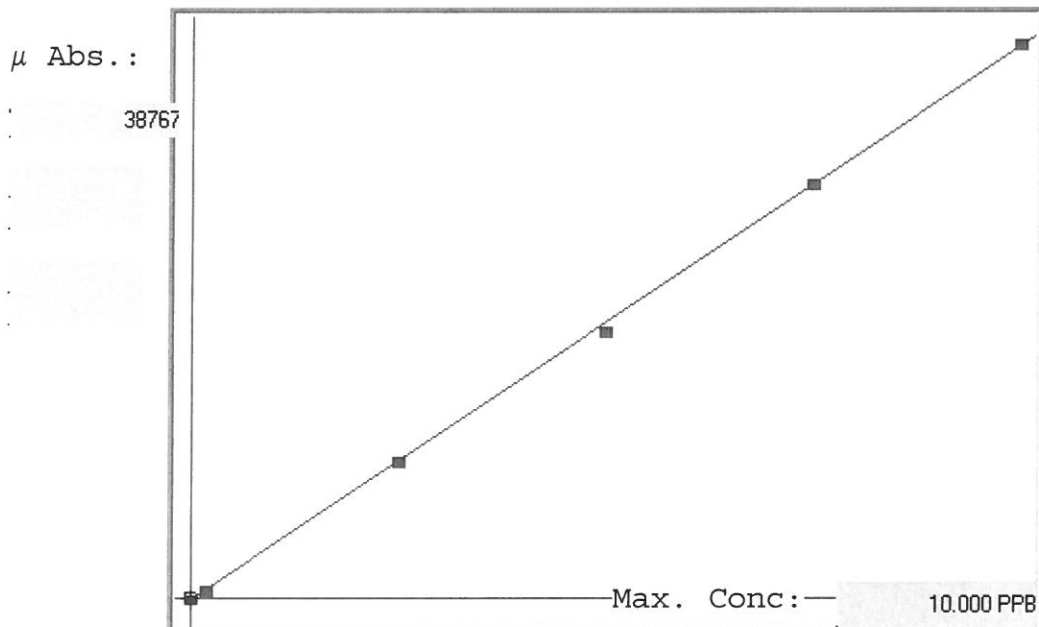

A= 0.0000e+000

B= 2.5810e-004

C= 3.6797e-002

Rho= 0.9998774

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.044	0.044	27	0.000	27				
0.2	0.200	0.203	0.003	643	0.0 %	643				
2.5	2.500	2.518	0.018	9614	0.0 %	9614				
5.0	5.000	4.875	-0.125	18745	0.0 %	18745				
7.5	7.500	7.518	0.018	28984	0.0 %	28984				
10.0	10.000	10.043	0.043	38767	0.0 %	38767				

LB96926 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 27 Jul 2018 10:33:29

Sample ID	Extended ID	μ Abs	Conc	Std ConcMethod	Units	Date	Type	Type
0.0 - 1	50	27	-	0.00007470A	PPB	27 Jul 2018 10:39:40	S	Std
0.2 - 1	50.2	643	-	0.20007470A	PPB	27 Jul 2018 10:41:48	S	Std
2.5 - 1	52.5	9614	-	2.50007470A	PPB	27 Jul 2018 10:43:57	S	Std
5.0 - 1	55	18745	-	5.00007470A	PPB	27 Jul 2018 10:46:05	S	Std
7.5 - 1	57.5	28984	-	7.50007470A	PPB	27 Jul 2018 10:48:13	S	Std
10.0 - 1	510	38767	-	10.00007470A	PPB	27 Jul 2018 10:50:20	S	Std
ICV74 - 1	ICV74	15079	3.9287	-7470A	PPB	27 Jul 2018 10:52:56	U	SMPL
ICB74 - 1	ICB74	-115	0.0071	-7470A	PPB	27 Jul 2018 10:55:02	U	SMPL
CCV25 - 1	CCV25	19324	5.0244	-7470A	PPB	27 Jul 2018 10:57:10	U	SMPL
CCB25 - 1	CCB25	-94	0.0125	-7470A	PPB	27 Jul 2018 10:59:17	U	SMPL
CRA - 1	CRA	652	0.2051	-7470A	PPB	27 Jul 2018 11:01:24	U	SMPL
HighStd - 1	HighStd	38454	9.9619	-7470A	PPB	27 Jul 2018 11:03:31	U	SMPL
ChkStd - 1	ChkStd	26500	6.8765	-7470A	PPB	27 Jul 2018 11:05:38	U	SMPL
PB111507BL - 1	PBW	-189	-0.0120	-7470A	PPB	27 Jul 2018 11:07:46	U	SMPL
PB111507BS - 1	LCSW	13653	3.5607	-7470A	PPB	27 Jul 2018 11:09:56	U	SMPL
PB111507TB - 1	PB111472TB	-68	0.0192	-7470A	PPB	27 Jul 2018 11:12:03	U	SMPL
J4152-04 - 1	LA-SOIL-1	28	0.0440	-7470A	PPB	27 Jul 2018 11:14:12	U	SMPL
J4152-04DUP - 1	LA-SOIL-1DUP	47	0.0489	-7470A	PPB	27 Jul 2018 11:16:20	U	SMPL
J4152-04MS - 1	LA-SOIL-1MS	13715	3.5767	-7470A	PPB	27 Jul 2018 11:18:29	U	SMPL
J4152-04MSD - 1	LA-SOIL-1MSD	13619	3.5519	-7470A	PPB	27 Jul 2018 11:20:35	U	SMPL
CCV26 - 1	CCV26	19343	5.0293	-7470A	PPB	27 Jul 2018 11:22:41	U	SMPL
CCB26 - 1	CCB26	-103	0.0102	-7470A	PPB	27 Jul 2018 11:24:48	U	SMPL
J4152-08 - 1	LA-SOIL-2	34	0.0456	-7470A	PPB	27 Jul 2018 11:26:55	U	SMPL
J4161-01 - 1	OILY-DEBRIS	137	0.0722	-7470A	PPB	27 Jul 2018 11:29:01	U	SMPL
J4161-02 - 1	OIL	384	0.1359	-7470A	PPB	27 Jul 2018 11:31:08	U	SMPL
J4162-07 - 1	NORTHLAWN-PRECHAR-AREA-3-B	127	0.0696	-7470A	PPB	27 Jul 2018 11:33:15	U	SMPL
PB111508BL - 1	PBW	97	0.0618	-7470A	PPB	27 Jul 2018 11:38:17	U	SMPL
PB111508BS - 1	LCSW	13782	3.5940	-7470A	PPB	27 Jul 2018 11:40:24	U	SMPL
PB111508TB - 1	PB111474TB	-33	0.0283	-7470A	PPB	27 Jul 2018 11:42:33	U	SMPL
J4158-02 - 1	OILY-WATER-TOTES	68	0.0543	-7470A	PPB	27 Jul 2018 11:44:40	U	SMPL
J4167-02 - 1	GS-OILY-WATER	90	0.0600	-7470A	PPB	27 Jul 2018 11:46:49	U	SMPL
J4167-02DUP - 1	GS-OILY-WATERDUP	84	0.0585	-7470A	PPB	27 Jul 2018 11:48:56	U	SMPL
CCV27 - 1	CCV27	18870	4.9072	-7470A	PPB	27 Jul 2018 11:51:03	U	SMPL
CCB27 - 1	CCB27	-76	0.0172	-7470A	PPB	27 Jul 2018 11:53:10	U	SMPL
J4167-02MS - 1	GS-OILY-WATERMS	14983	3.9040	-7470A	PPB	27 Jul 2018 11:55:17	U	SMPL
J4167-02MSD - 1	GS-OILY-WATERMSD	13920	3.6296	-7470A	PPB	27 Jul 2018 11:57:24	U	SMPL
PB111509BL - 1	PBW	-36	0.0275	-7470A	PPB	27 Jul 2018 11:59:31	U	SMPL
PB111509BS - 1	LCSW	13325	3.4760	-7470A	PPB	27 Jul 2018 12:01:39	U	SMPL
J4070-04 - 1	LC-SD-EB02-180718	-169	-0.0068	-7470A	PPB	27 Jul 2018 12:03:46	U	SMPL
J4154-11 - 1	FL-EB-2018-1	-140	0.0007	-7470A	PPB	27 Jul 2018 12:05:54	U	SMPL
J4158-01 - 1	OILY-WATER-TOTES	6209	1.6394	-7470A	PPB	27 Jul 2018 12:08:02	U	SMPL
J4164-12 - 1	FB-072518	-153	-0.0027	-7470A	PPB	27 Jul 2018 12:10:10	U	SMPL
J4167-01 - 1	GS-OILY-WATER	-11	0.0340	-7470A	PPB	27 Jul 2018 12:12:19	U	SMPL
J4167-01DUP - 1	GS-OILY-WATERDUP	-14	0.0332	-7470A	PPB	27 Jul 2018 12:14:27	U	SMPL
CCV28 - 1	CCV28	18494	4.8102	-7470A	PPB	27 Jul 2018 12:16:34	U	SMPL
CCB28 - 1	CCB28	34	0.0456	-7470A	PPB	27 Jul 2018 12:23:43	U	SMPL
J4167-01MS - 1	GS-OILY-WATERMS	14435	3.7625	-7470A	PPB	27 Jul 2018 12:25:49	U	SMPL
J4167-01MSD - 1	GS-OILY-WATERMSD	13584	3.5429	-7470A	PPB	27 Jul 2018 12:27:57	U	SMPL
J4176-01 - 1	SV26835	2773	0.7525	-7470A	PPB	27 Jul 2018 12:30:05	U	SMPL
J4188-01 - 1	HA-BASELINEWATER-N48971	-100	0.0110	-7470A	PPB	27 Jul 2018 12:32:13	U	SMPL
J4189-26 - 1	TP-12	53603	13.8719	-7470A	PPB	27 Jul 2018 12:34:20	U	SMPL
J4104-04 - 1	LC-SD-EB03-180719	-165	-0.0058	-7470A	PPB	27 Jul 2018 12:43:07	U	SMPL
CCV29 - 1	CCV29	17864	4.6476	-7470A	PPB	27 Jul 2018 12:45:14	U	SMPL
CCB29 - 1	CCB29	-30	0.0291	-7470A	PPB	27 Jul 2018 12:49:53	U	SMPL
J4152-04LX5 - 1		-30	0.0291	-7470A	PPB	27 Jul 2018 12:52:02	U	SMPL
J4152-04A - 1		14225	3.7083	-7470A	PPB	27 Jul 2018 12:54:09	U	SMPL
J4167-02LX5 - 1		-95	0.0123	-7470A	PPB	27 Jul 2018 12:56:16	U	SMPL
J4167-02A - 1		14564	3.7958	-7470A	PPB	27 Jul 2018 12:58:23	U	SMPL
J4167-01LX5 - 1		-122	0.0053	-7470A	PPB	27 Jul 2018 13:00:30	U	SMPL
J4167-01A - 1		15669	4.0810	-7470A	PPB	27 Jul 2018 13:02:37	U	SMPL
J4189-26DLX2 - 1		25390	6.5900	-7470A	PPB	27 Jul 2018 13:04:44	U	SMPL
CCV30 - 1	CCV30	18693	4.8615	-7470A	PPB	27 Jul 2018 13:06:52	U	SMPL
CCB30 - 1	CCB30	-75	0.0174	-7470A	PPB	27 Jul 2018 13:09:01	U	SMPL