


7471B

L396945
INSTRUMENT ID: CV1

Linear

 μ Abs.:

44165

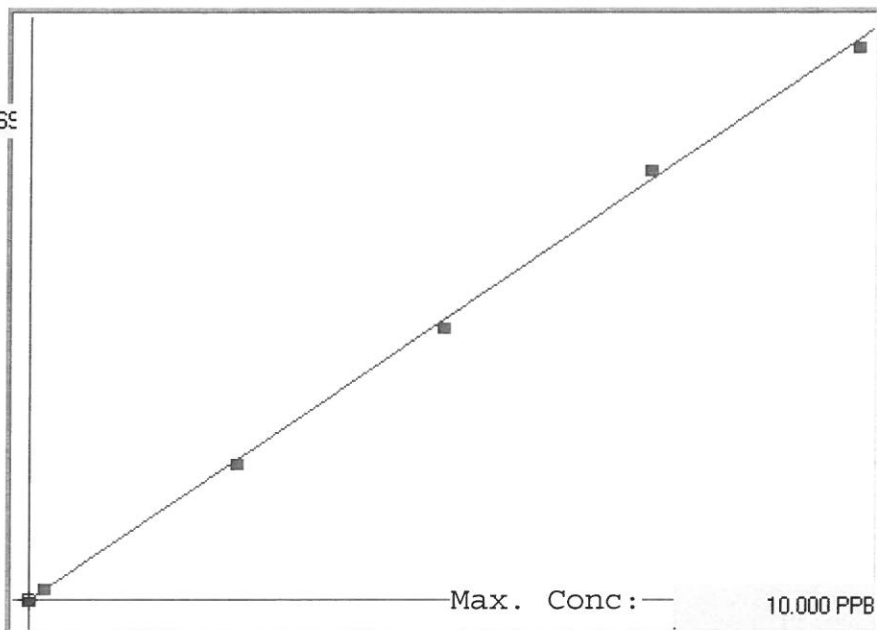

A= 0.0000e+000

B= 2.2389e-004

C= 1.9671e-002

Rho= 0.9995808

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.019	0.019	-4	0.000	-4				
0.2	0.200	0.230	0.030	939	0.0 %	939				
2.5	2.500	2.456	-0.044	10883	0.0 %	10883				
5.0	5.000	4.880	-0.120	21708	0.0 %	21708				
7.5	7.500	7.706	0.206	34332	0.0 %	34332				
10.0	10.000	9.909	-0.091	44169	0.0 %	44169				

LB96945 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 27 Jul 2018 16:36:41

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	80	-4	-	0.0000	7471B	PPB	27 Jul 2018 16:39:01	S	Std
0.2 - 1	50.2	939	-	0.2000	7471B	PPB	27 Jul 2018 16:41:18	S	Std
2.5 - 1	52.5	10883	-	2.5000	7471B	PPB	27 Jul 2018 16:43:36	S	Std
5.0 - 1	55	21708	-	5.0000	7471B	PPB	27 Jul 2018 16:45:54	S	Std
7.5 - 1	57.5	34332	-	7.5000	7471B	PPB	27 Jul 2018 16:48:11	S	Std
10.0 - 1	510	44169	-	10.0000	7471B	PPB	27 Jul 2018 16:53:10	S	Std
ICV76 - 1	ICV76	18035	4.0576	-	7471B	PPB	27 Jul 2018 16:55:53	U	SMPL
ICB76 - 1	ICB76	-284	-0.0439	-	7471B	PPB	27 Jul 2018 16:58:09	U	SMPL
CCV35 - 1	CCV35	22220	4.9946	-	7471B	PPB	27 Jul 2018 17:00:25	U	SMPL
CCB35 - 1	CCB35	-246	-0.0354	-	7471B	PPB	27 Jul 2018 17:02:41	U	SMPL
CRA - 1	CRA	909	0.2232	-	7471B	PPB	27 Jul 2018 17:04:59	U	SMPL
HighStd - 1	HighStd	44372	9.9542	-	7471B	PPB	27 Jul 2018 17:07:14	U	SMPL
ChkStd - 1	ChkStd	31784	7.1359	-	7471B	PPB	27 Jul 2018 17:09:31	U	SMPL
PB111515BL - 1	PBS	-391	-0.0679	-	7471B	PPB	27 Jul 2018 17:11:50	U	SMPL
PB111515BS - 1	LCSS	16876	3.7981	-	7471B	PPB	27 Jul 2018 17:14:09	U	SMPL
J4176-04 - 1	PLASTIC-COAT	6754	1.5318	-	7471B	PPB	27 Jul 2018 17:16:25	U	SMPL
J4180-01 - 1	GS-PIT-1	6336	1.4383	-	7471B	PPB	27 Jul 2018 17:18:43	U	SMPL
J4180-05 - 1	GS-PIT-2	1755	0.4126	-	7471B	PPB	27 Jul 2018 17:21:02	U	SMPL
J4189-03 - 1	TP-12-S	10260	2.3168	-	7471B	PPB	27 Jul 2018 17:23:20	U	SMPL
J4189-07 - 1	TP-12-D	1472	0.3492	-	7471B	PPB	27 Jul 2018 17:25:36	U	SMPL
CCV36 - 1	CCV36	22088	4.9650	-	7471B	PPB	27 Jul 2018 17:27:52	U	SMPL
CCB36 - 1	CCB36	-194	-0.0238	-	7471B	PPB	27 Jul 2018 17:30:07	U	SMPL
J4189-11 - 1	TP-13-S	6408	1.4544	-	7471B	PPB	27 Jul 2018 17:32:23	U	SMPL
J4189-15 - 1	TP-14-S	12422	2.8009	-	7471B	PPB	27 Jul 2018 17:34:39	U	SMPL
J4189-19 - 1	TP-14-D	1344	0.3206	-	7471B	PPB	27 Jul 2018 17:36:55	U	SMPL
J4192-01 - 1	FK-BPM-03-001-A	1182	0.2843	-	7471B	PPB	27 Jul 2018 17:39:12	U	SMPL
J4192-01DUP - 1	FK-BPM-03-001-ADUP	1200	0.2883	-	7471B	PPB	27 Jul 2018 17:41:29	U	SMPL
J4192-01MS - 1	FK-BPM-03-001-AMS	17826	4.0108	-	7471B	PPB	27 Jul 2018 17:43:46	U	SMPL
J4192-01MSD - 1	FK-BPM-03-001-AMSD	17748	3.9933	-	7471B	PPB	27 Jul 2018 17:46:03	U	SMPL
J4192-03 - 1	FK-BPM-03-001-B	1296	0.3098	-	7471B	PPB	27 Jul 2018 17:48:20	U	SMPL
J4192-05 - 1	FK-BPM-03-001-C	831	0.2057	-	7471B	PPB	27 Jul 2018 17:50:38	U	SMPL
J4192-07 - 1	FK-BPM-03-001-D	1479	0.3508	-	7471B	PPB	27 Jul 2018 17:52:54	U	SMPL
CCV37 - 1	CCV37	22271	5.0060	-	7471B	PPB	27 Jul 2018 17:55:11	U	SMPL
CCB37 - 1	CCB37	-203	-0.0258	-	7471B	PPB	27 Jul 2018 17:57:27	U	SMPL
J4193-01 - 1	FK-PS-01-035	963	0.2353	-	7471B	PPB	27 Jul 2018 17:59:43	U	SMPL
J4192-01LX5 - 1		70	0.0353	-	7471B	PPB	27 Jul 2018 18:01:59	U	SMPL
J4192-01A - 1		18802	4.2293	-	7471B	PPB	27 Jul 2018 18:04:16	U	SMPL
CCV38 - 1	CCV38	22381	5.0306	-	7471B	PPB	27 Jul 2018 18:06:32	U	SMPL
CCB38 - 1	CCB38	-230	-0.0318	-	7471B	PPB	27 Jul 2018 18:08:49	U	SMPL