


ISM02.4

LB 96972
INSTRUMENT ID: CX4

Linear

 μ Abs.:

43077

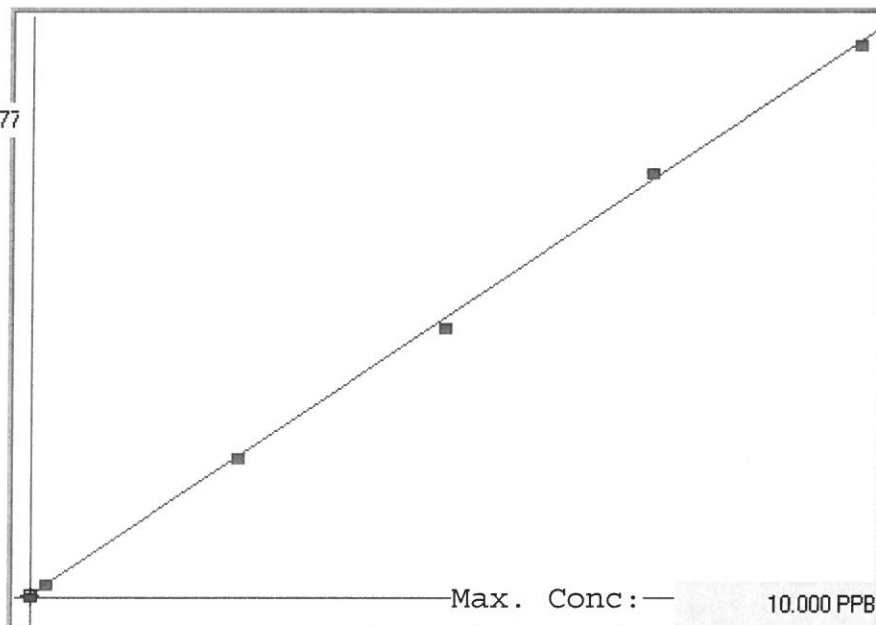

A= 0.0000e+000

B= 2.3182e-004

C= -3.9176e-002

Rho= 0.9997228

Accept=Accepted

slope
 $y = 10150 \cdot x$

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.00	0.000	0.002	0.002	178	0.000	178				
0.2	0.200	0.223	0.023	1129	0.0 %	1129				
2.5	2.500	2.516	0.016	11020	0.0 %	11020				
5.0	5.000	4.862	-0.138	21142	0.0 %	21142				
7.5	7.500	7.651	0.151	33171	0.0 %	33171				
10.0	10.000	9.947	-0.053	43077	0.0 %	43077				

0/0 D

12

-1

-3

2

-1

103

7/30/18

INSTRUMENT ID : CV1

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type
	0 S0.0	178	-		0 ISM02.4	PPB	7/30/2018 14:07	Std
	0.2 S0.2	1129	-		0.2 ISM02.4	PPB	7/30/2018 14:09	Std
	2.5 S2.5	11020	-		2.5 ISM02.4	PPB	7/30/2018 14:11	Std
	5 S5	21142	-		5 ISM02.4	PPB	7/30/2018 14:14	Std
	7.5 S7.5	33171	-		7.5 ISM02.4	PPB	7/30/2018 14:16	Std
	10 S10.0	43077	-		10 ISM02.4	PPB	7/30/2018 14:24	Std
ICV	ICV	16860	3.8694 -		ISM02.4	PPB	7/30/2018 14:26	SMPL
ICB	ICB	-41	-0.0487 -		ISM02.4	PPB	7/30/2018 14:29	SMPL
CCV044	CCV044	21380	4.9172 -		ISM02.4	PPB	7/30/2018 14:31	SMPL
CCB044	CCB044	-59	-0.0529 -		ISM02.4	PPB	7/30/2018 14:33	SMPL
PB111566BL	PBW003	-62	-0.0535 -		ISM02.4	PPB	7/30/2018 14:35	SMPL
J4201-01	MBE719	100	-0.016 -		ISM02.4	PPB	7/30/2018 14:38	SMPL
J4201-02	MBE719D	78	-0.0211 -		ISM02.4	PPB	7/30/2018 14:40	SMPL
J4201-03	MBE719S	4946	1.1074 -		ISM02.4	PPB	7/30/2018 14:42	SMPL
CCV045	CCV045	20859	4.7964 -		ISM02.4	PPB	7/30/2018 14:44	SMPL
CCB045	CCB045	-72	-0.0559 -		ISM02.4	PPB	7/30/2018 14:47	SMPL