


7470A

LB 97123
INSTRUMENT ID: C41

Linear

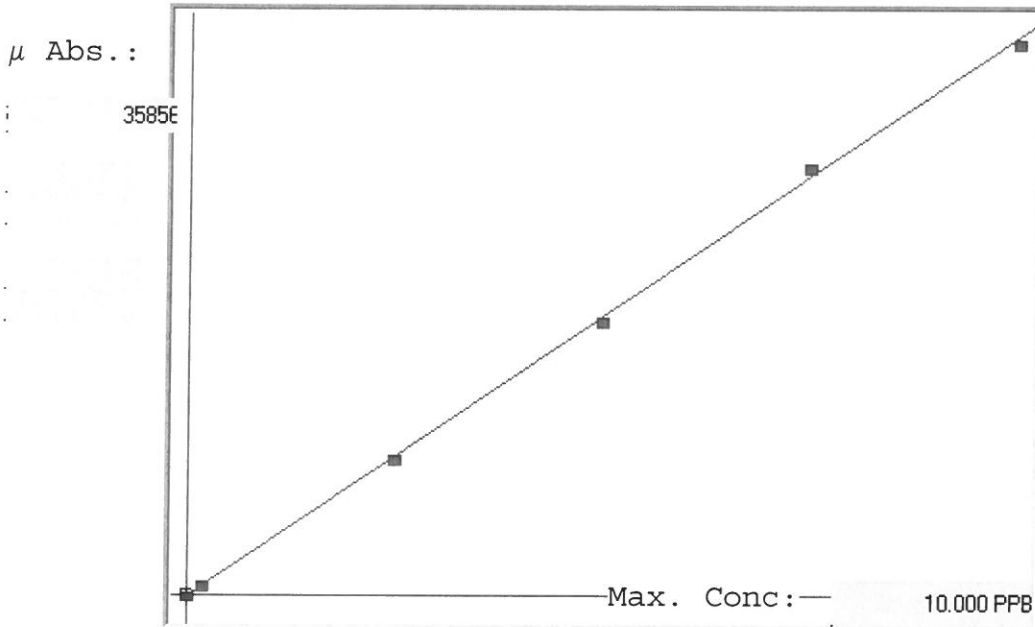

A= 0.0000e+000

B= 2.7557e-004

C= 2.5760e-002

Rho= 0.9997249

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.015	0.015	-38	0.000	-38				
0.2	0.200	0.208	0.008	661	0.0 %	661				
2.5	2.500	2.460	-0.040	8832	0.0 %	8832				
5.0	5.000	4.936	-0.064	17820	0.0 %	17820				
7.5	7.500	7.674	0.174	27754	0.0 %	27754				
10.0	10.000	9.907	-0.093	35856	0.0 %	35856				

LB97123 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 06 Aug 2018 09:22:14

Sample ID	Extended ID	µ Abs	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-38	-	0.0000	7470A	PPB	06 Aug 2018 09:26:28	S	Std
0.2 - 1	50.2	661	-	0.2000	7470A	PPB	06 Aug 2018 09:28:36	S	Std
2.5 - 1	52.5	8832	-	2.5000	7470A	PPB	06 Aug 2018 09:30:45	S	Std
5.0 - 1	55	17820	-	5.0000	7470A	PPB	06 Aug 2018 09:32:53	S	Std
7.5 - 1	57.5	27754	-	7.5000	7470A	PPB	06 Aug 2018 09:35:01	S	Std
10.0 - 1	510	35856	-	10.0000	7470A	PPB	06 Aug 2018 09:37:08	S	Std
ICV89 - 1	ICV89	14064	3.9014	-	7470A	PPB	06 Aug 2018 09:39:47	U	SMPL
ICB89 - 1	ICB89	-224	-0.0360	-	7470A	PPB	06 Aug 2018 09:41:53	U	SMPL
CCV01 - 1	CCV01	18629	5.1594	-	7470A	PPB	06 Aug 2018 09:44:01	U	SMPL
CCB01 - 1	CCB01	-249	-0.0429	-	7470A	PPB	06 Aug 2018 09:46:07	U	SMPL
CRA - 1	CRA	641	0.2024	-	7470A	PPB	06 Aug 2018 09:48:15	U	SMPL
HighStd - 1	HighStd	36211	10.0045	-	7470A	PPB	06 Aug 2018 09:50:21	U	SMPL
ChkStd - 1	ChkStd	24141	6.6784	-	7470A	PPB	06 Aug 2018 09:52:28	U	SMPL
PB111753BL - 1	PBW	-382	-0.0795	-	7470A	PPB	06 Aug 2018 09:54:37	U	SMPL
PB111753BS - 1	LCSW	13785	3.8245	-	7470A	PPB	06 Aug 2018 09:56:46	U	SMPL
PB111753TB - 1	PB111718TB	-192	-0.0272	-	7470A	PPB	06 Aug 2018 09:58:53	U	SMPL
J4310-02 - 1	C-1	-102	-0.0023	-	7470A	PPB	06 Aug 2018 10:01:01	U	SMPL
J4310-02DUP - 1	C-1DUP	-75	0.0051	-	7470A	PPB	06 Aug 2018 10:03:10	U	SMPL
J4310-02MS - 1	C-1MS	12829	3.5611	-	7470A	PPB	06 Aug 2018 10:05:18	U	SMPL
J4310-02MSD - 1	C-1MSD	13595	3.7722	-	7470A	PPB	06 Aug 2018 10:07:25	U	SMPL
CCV02 - 1	CCV02	18473	5.1164	-	7470A	PPB	06 Aug 2018 10:09:32	U	SMPL
CCB02 - 1	CCB02	-251	-0.0434	-	7470A	PPB	06 Aug 2018 10:11:39	U	SMPL
J4310-04 - 1	C-2	-77	0.0045	-	7470A	PPB	06 Aug 2018 10:13:47	U	SMPL
J4310-06 - 1	C-3	-45	0.0134	-	7470A	PPB	06 Aug 2018 10:15:53	U	SMPL
J4310-08 - 1	C-4	-40	0.0147	-	7470A	PPB	06 Aug 2018 10:18:00	U	SMPL
J4313-02 - 1	C-5	-43	0.0139	-	7470A	PPB	06 Aug 2018 10:20:07	U	SMPL
J4313-04 - 1	C-6	-69	0.0067	-	7470A	PPB	06 Aug 2018 10:22:15	U	SMPL
J4313-06 - 1	C-7	-91	0.0007	-	7470A	PPB	06 Aug 2018 10:24:23	U	SMPL
J4313-08 - 1	C-8	-48	0.0125	-	7470A	PPB	06 Aug 2018 10:26:31	U	SMPL
J4313-10 - 1	C-9	-41	0.0145	-	7470A	PPB	06 Aug 2018 10:28:39	U	SMPL
J4313-12 - 1	C-10	-39	0.0150	-	7470A	PPB	06 Aug 2018 10:30:48	U	SMPL
J4313-14 - 1	C-11	-45	0.0134	-	7470A	PPB	06 Aug 2018 10:32:54	U	SMPL
CCV03 - 1	CCV03	18252	5.0555	-	7470A	PPB	06 Aug 2018 10:35:01	U	SMPL
CCB03 - 1	CCB03	-216	-0.0338	-	7470A	PPB	06 Aug 2018 10:37:08	U	SMPL
J4313-16 - 1	C-12	-76	0.0048	-	7470A	PPB	06 Aug 2018 10:39:17	U	SMPL
J4313-18 - 1	C-13	-43	0.0139	-	7470A	PPB	06 Aug 2018 10:41:24	U	SMPL
J4313-20 - 1	C-14	-28	0.0180	-	7470A	PPB	06 Aug 2018 10:43:31	U	SMPL
J4318-02 - 1	BEEBEE-SITE-DEMO-1	-40	0.0147	-	7470A	PPB	06 Aug 2018 10:45:38	U	SMPL
J4318-04 - 1	BEEBEE-SITE-DEMO-2	3	0.0266	-	7470A	PPB	06 Aug 2018 10:47:46	U	SMPL
J4318-06 - 1	BEEBEE-SITE-DEMO-2A	-35	0.0161	-	7470A	PPB	06 Aug 2018 10:49:54	U	SMPL
J4318-08 - 1	BEEBEE-SITE-DEMO-3	-60	0.0092	-	7470A	PPB	06 Aug 2018 10:52:02	U	SMPL
J4318-10 - 1	BEEBEE-SITE-DEMO-4	-15	0.0216	-	7470A	PPB	06 Aug 2018 10:54:10	U	SMPL
J4318-12 - 1	BEEBEE-SITE-DEMO-5	-58	0.0098	-	7470A	PPB	06 Aug 2018 10:56:18	U	SMPL
PB111754BL - 1	PBW	-51	0.0117	-	7470A	PPB	06 Aug 2018 10:58:25	U	SMPL
CCV04 - 1	CCV04	18335	5.0784	-	7470A	PPB	06 Aug 2018 11:00:32	U	SMPL
CCB04 - 1	CCB04	-211	-0.0324	-	7470A	PPB	06 Aug 2018 11:02:39	U	SMPL
PB111754BS - 1	LCSW	13661	3.7904	-	7470A	PPB	06 Aug 2018 11:04:48	U	SMPL
PB111754TB - 1	PB111725TB	-187	-0.0258	-	7470A	PPB	06 Aug 2018 11:06:55	U	SMPL
J4298-04 - 1	WC-3	-73	0.0056	-	7470A	PPB	06 Aug 2018 11:09:02	U	SMPL
J4298-04DUP - 1	WC-3DUP	-15	0.0216	-	7470A	PPB	06 Aug 2018 11:11:09	U	SMPL
J4298-04MS - 1	WC-3MS	13925	3.8631	-	7470A	PPB	06 Aug 2018 11:13:16	U	SMPL
J4298-04MSD - 1	WC-3MSD	14356	3.9819	-	7470A	PPB	06 Aug 2018 11:15:24	U	SMPL
J4316-04 - 1	T40-STONE-1	-200	-0.0294	-	7470A	PPB	06 Aug 2018 11:17:32	U	SMPL
J4316-08 - 1	T40-CLAY-1	-63	0.0084	-	7470A	PPB	06 Aug 2018 11:19:41	U	SMPL
J4323-02 - 1	ES-RO-276	-60	0.0092	-	7470A	PPB	06 Aug 2018 11:21:50	U	SMPL
PB111755BL - 1	PBW	-59	0.0095	-	7470A	PPB	06 Aug 2018 11:23:57	U	SMPL
CCV05 - 1	CCV05	18636	5.1613	-	7470A	PPB	06 Aug 2018 11:26:04	U	SMPL
CCB05 - 1	CCB05	-197	-0.0285	-	7470A	PPB	06 Aug 2018 11:28:11	U	SMPL
PB111755BS - 1	LCSW	13788	3.8254	-	7470A	PPB	06 Aug 2018 11:30:19	U	SMPL
PB111755TB - 1	PB111726TB	-140	-0.0128	-	7470A	PPB	06 Aug 2018 11:32:27	U	SMPL
J4316-10 - 1	OW-2-4	-49	0.0123	-	7470A	PPB	06 Aug 2018 11:34:34	U	SMPL
J4316-10DUP - 1	OW-2-4DUP	-40	0.0147	-	7470A	PPB	06 Aug 2018 11:36:41	U	SMPL
J4316-10MS - 1	OW-2-4MS	14058	3.8998	-	7470A	PPB	06 Aug 2018 11:38:48	U	SMPL
J4316-10MSD - 1	OW-2-4MSD	14996	4.1583	-	7470A	PPB	06 Aug 2018 11:40:56	U	SMPL
J4317-02 - 1	N28424	-197	-0.0285	-	7470A	PPB	06 Aug 2018 11:43:04	U	SMPL
PB111756BL - 1	PBW	34	0.0351	-	7470A	PPB	06 Aug 2018 11:45:13	U	SMPL
PB111756BS - 1	LCSW	13626	3.7807	-	7470A	PPB	06 Aug 2018 11:47:22	U	SMPL
J4316-09 - 1	OW-2-4	680	0.2131	-	7470A	PPB	06 Aug 2018 11:49:29	U	SMPL
CCV06 - 1	CCV06	18303	5.0696	-	7470A	PPB	06 Aug 2018 11:51:37	U	SMPL
CCB06 - 1	CCB06	-190	-0.0266	-	7470A	PPB	06 Aug 2018 11:53:45	U	SMPL
J4316-09DUP - 1	OW-2-4DUP	607	0.1930	-	7470A	PPB	06 Aug 2018 11:55:18	U	SMPL
J4316-09MS - 1	OW-2-4MS	15223	4.2208	-	7470A	PPB	06 Aug 2018 12:00:24	U	SMPL
J4316-09MSD - 1	OW-2-4MSD	16491	4.5702	-	7470A	PPB	06 Aug 2018 12:02:32	U	SMPL
J4317-01 - 1	N28424	-207	-0.0313	-	7470A	PPB	06 Aug 2018 12:04:41	U	SMPL
CCV07 - 1	CCV07	18200	5.0412	-	7470A	PPB	06 Aug 2018 12:06:49	U	SMPL
CCB07 - 1	CCB07	-172	-0.0216	-	7470A	PPB	06 Aug 2018 12:08:57	U	SMPL
J4310-02LX5 - 1		-28	0.0180	-	7470A	PPB	06 Aug 2018 12:11:07	U	SMPL
J4310-02A - 1		11952	3.3194	-	7470A	PPB	06 Aug 2018 12:13:15	U	SMPL
J4298-04LX5 - 1		-111	-0.0048	-	7470A	PPB	06 Aug 2018 12:15:23	U	SMPL
J4298-04A - 1		11904	3.3062	-	7470A	PPB	06 Aug 2018 12:17:31	U	SMPL
J4316-10LX5 - 1		-172	-0.0216	-	7470A	PPB	06 Aug 2018 12:19:38	U	SMPL

LB97123 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 06 Aug 2018 09:22:14

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
J4316-10A - 1		11645	3.2348		-7470A	PPB	06 Aug 2018 12:21:46	U	SMPL
J4316-09LX5 - 1		36	0.0357		-7470A	PPB	06 Aug 2018 12:23:53	U	SMPL
J4316-09A - 1		16242	4.5016		-7470A	PPB	06 Aug 2018 12:26:01	U	SMPL
CCV08 - 1	CCV08	18105	5.0150		-7470A	PPB	06 Aug 2018 12:28:09	U	SMPL
CCB08 - 1	CCB08	-251	-0.0434		-7470A	PPB	06 Aug 2018 12:30:18	U	SMPL